

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alexander Instrument Location Alexander Co 50

Instrument Serial No. 008060 Taylorsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1049
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALEXANDER COUNTY ALEXANDER COUNTY SO
010

Serial Number: 008660

Test Date: 02/08/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	5:13pm
AIR BLK	.00	5:14pm
ACCY CHK	.08	5:15pm
AIR BLK	.00	5:16pm
SUB TEST	.00	5:17pm
AIR BLK	.00	5:18pm
SUB TEST	.00	5:19pm
AIR BLK	.00	5:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ALEXANDER COUNTY ALEXANDER COUNTY SO 010

Serial Number: 008660 Test Record Number: 4451
Test Date: 02/08/2022 Test Time: 5:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:22pm
FLO	Pass	5:22pm
FC	Pass	5:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:22pm
SRC	Pass	5:22pm
DET	Pass	5:22pm
BAR	Pass	5:22pm
BT	Pass	5:22pm

Blank Tests

Test	Status	Time
AIR	Pass	5:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:23pm

CRC Tests

Test	Status	Time
COMP	Pass	5:23pm
CAL	Pass	5:23pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alexander Instrument Location Alexander Co SO
Instrument Serial No. 008813 Taylorsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALEXANDER COUNTY ALEXANDER COUNTY SO
010

Serial Number: 008813
Test Date: 02/07/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	2:58pm
AIR BLK	.00	2:59pm
ACCY CHK	.08	3:00pm
AIR BLK	.00	3:01pm
SUB TEST	.00	3:02pm
AIR BLK	.00	3:03pm
SUB TEST	.00	3:04pm
AIR BLK	.00	3:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ALEXANDER COUNTY ALEXANDER COUNTY SO 010

Serial Number: 008813 Test Record Number: 2141
Test Date: 02/07/2022 Test Time: 3:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:06pm
FLO	Pass	3:06pm
FC	Pass	3:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:06pm
SRC	Pass	3:06pm
DET	Pass	3:06pm
BAR	Pass	3:06pm
BT	Pass	3:06pm

Blank Tests

Test	Status	Time
AIR	Pass	3:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:07pm

CRC Tests

Test	Status	Time
COMP	Pass	3:07pm
CAL	Pass	3:07pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Allegheny Instrument Location Allegheny Co Jail
Instrument Serial No. 008890 Sparta, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890

Test Date: 02/14/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENACE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	1:26pm
AIR BLK	.00	1:27pm
ACCY CHK	.07	1:28pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:29pm
AIR BLK	.00	1:30pm
SUB TEST	.00	1:32pm
AIR BLK	.00	1:33pm

Reported AC: .00 g/210L

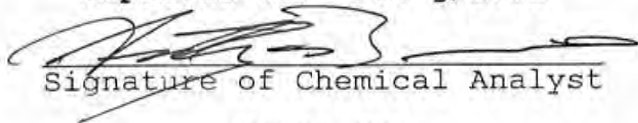

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890 Test Record Number: 873
Test Date: 02/14/2022 Test Time: 1:34pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:34pm
FLO	Pass	1:34pm
FC	Pass	1:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:35pm
SRC	Pass	1:35pm
DET	Pass	1:35pm
BAR	Pass	1:35pm
BT	Pass	1:35pm

Blank Tests

Test	Status	Time
AIR	Pass	1:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:35pm

CRC Tests

Test	Status	Time
COMP	Pass	1:35pm
CAL	Pass	1:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Ashe Instrument Location Ashe Co Jail
Instrument Serial No. 008849 Jefferson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ASHE COUNTY ASHE COUNTY JAIL 040

Serial Number: 008849

Test Date: 02/14/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	3:28pm
AIR BLK	.00	3:28pm
ACCY CHK	.08	3:29pm
AIR BLK	.00	3:30pm
SUB TEST	.00	3:31pm
AIR BLK	.00	3:32pm
SUB TEST	.00	3:33pm
AIR BLK	.00	3:34pm

Reported AC: .00 g/210L

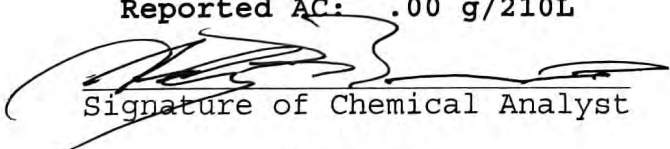
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ASHE COUNTY ASHE COUNTY JAIL 040

Serial Number: 008849 Test Record Number: 1518
Test Date: 02/14/2022 Test Time: 3:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:35pm
FLO	Pass	3:35pm
FC	Pass	3:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:36pm
SRC	Pass	3:36pm
DET	Pass	3:36pm
BAR	Pass	3:36pm
BT	Pass	3:36pm

Blank Tests

Test	Status	Time
AIR	Pass	3:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:36pm

CRC Tests

Test	Status	Time
COMP	Pass	3:37pm
CAL	Pass	3:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Avery Instrument Location Banner Elk PO
Instrument Serial No. 008724 Banner Elk, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724

Test Date: 02/14/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107502

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	10:06am
AIR BLK	.00	10:07am
ACCY CHK	.08	10:08am
AIR BLK	.00	10:09am
SUB TEST	.00	10:09am
AIR BLK	.00	10:10am
SUB TEST	.00	10:12am
AIR BLK	.00	10:13am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724 Test Record Number: 702
Test Date: 02/14/2022 Test Time: 10:14am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:15am
FLO	Pass	10:15am
FC	Pass	10:15am

Temperature Tests

Test	Status	Time
FC1	Pass	10:15am
SRC	Pass	10:15am
DET	Pass	10:15am
BAR	Pass	10:15am
BT	Pass	10:15am

Blank Tests

Test	Status	Time
AIR	Pass	10:15am

Printer Tests

Test	Status	Time
PRNT	Pass	10:15am

CRC Tests

Test	Status	Time
COMP	Pass	10:16am
CAL	Pass	10:16am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Bertie Instrument Location Bertie Co. S.O.
Instrument Serial No. 008897 232 County Farm Rd, Windsor, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BERTIE COUNTY BERTIE CO SO 070

Serial Number: 008897
Test Date: 02/09/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034901

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	11:55am
AIR BLK	.00	11:55am
ACCY CHK	.07	11:56am
AIR BLK	.00	11:57am
SUB TEST	.00	11:58am
AIR BLK	.00	11:59am
SUB TEST	.00	12:01pm
AIR BLK	.00	12:01pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BERTIE COUNTY BERTIE CO SO 070

Serial Number: 008897 Test Record Number: 1437
Test Date: 02/09/2022 Test Time: 12:02pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:03pm
FLO	Pass	12:03pm
FC	Pass	12:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:03pm
SRC	Pass	12:03pm
DET	Pass	12:03pm
BAR	Pass	12:03pm
BT	Pass	12:03pm

Blank Tests

Test	Status	Time
AIR	Pass	12:03pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:03pm

CRC Tests

Test	Status	Time
COMP	Pass	12:04pm
CAL	Pass	12:04pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location Buncombe County Detention
Instrument Serial No. 006748 Asheville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1069
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BUNCOMBE COUNTY JAIL
100

Serial Number: 008748
Test Date: 02/03/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG132001
Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	11:34am
AIR BLK	.00	11:35am
ACCY CHK	.07	11:35am
AIR BLK	.00	11:37am
SUB TEST	.00	11:38am
AIR BLK	.00	11:39am
SUB TEST	.00	11:40am
AIR BLK	.00	11:41am

Reported AC: .00 g/210L

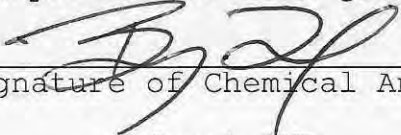

Signature of Chemical Analyst
Court CVR

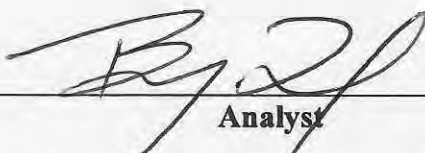

Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BUNCOMBE COUNTY JAIL 100

Serial Number: 008748 Test Record Number: 1670
Test Date: 02/03/2022 Test Time: 11:41am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:42am
FLO	Pass	11:42am
FC	Pass	11:42am

Temperature Tests

Test	Status	Time
FC1	Pass	11:42am
SRC	Pass	11:42am
DET	Pass	11:42am
BAR	Pass	11:42am
BT	Pass	11:42am

Blank Tests

Test	Status	Time
AIR	Pass	11:42am

Printer Tests

Test	Status	Time
PRNT	Pass	11:43am

CRC Tests

Test	Status	Time
COMP	Pass	11:43am
CAL	Pass	11:43am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location Buncombe County Detention
Instrument Serial No. 005798 Ashville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1068
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BUNCOMBE COUNTY JAIL
100

Serial Number: 008798
Test Date: 02/03/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	11:36am
AIR BLK	.00	11:36am
ACCY CHK	.07	11:37am
AIR BLK	.00	11:38am
SUB TEST	.00	11:39am
AIR BLK	.00	11:40am
SUB TEST	.00	11:41am
AIR BLK	.00	11:42am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BUNCOMBE COUNTY JAIL 100

Serial Number: 008798 Test Record Number: 5969
Test Date: 02/03/2022 Test Time: 11:44am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:44am
FLO	Pass	11:44am
FC	Pass	11:44am

Temperature Tests

Test	Status	Time
FC1	Pass	11:44am
SRC	Pass	11:44am
DET	Pass	11:44am
BAR	Pass	11:44am
BT	Pass	11:44am

Blank Tests

Test	Status	Time
AIR	Pass	11:45am

Printer Tests

Test	Status	Time
PRNT	Pass	11:45am

CRC Tests

Test	Status	Time
COMP	Pass	11:45am
CAL	Pass	11:45am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Kannapolis PD
Instrument Serial No. 008589 Kannapolis, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

KANNAPOLIS PD CABARRUS COUNTY 120

Serial Number: 008589

Test Date: 02/09/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132001

Exp Date: 11/16/2022

Test	g/210L	Time
DIAG	Pass	12:41pm
AIR BLK	.00	12:42pm
ACCY CHK	.07	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:44pm
AIR BLK	.00	12:45pm
SUB TEST	.00	12:46pm
AIR BLK	.00	12:47pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

KANNAPOLIS PD CABARRUS COUNTY 120

Serial Number: 008589 Test Record Number: 3361
Test Date: 02/09/2022 Test Time: 12:49pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:49pm
FLO	Pass	12:49pm
FC	Pass	12:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:49pm
SRC	Pass	12:49pm
DET	Pass	12:49pm
BAR	Pass	12:49pm
BT	Pass	12:49pm

Blank Tests

Test	Status	Time
AIR	Pass	12:50pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:50pm

CRC Tests

Test	Status	Time
COMP	Pass	12:50pm
CAL	Pass	12:50pm

Preventive Maintenance
Status: Pass

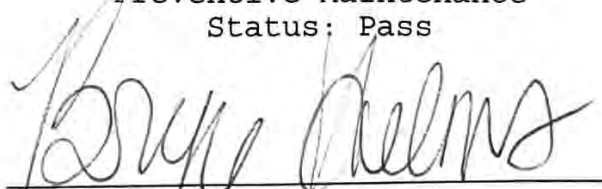

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CASWELL Instrument Location CASWELL Co Detention Ctr
Instrument Serial No. 008593 211 County Park Rd
Yanceyville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

602
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593

Test Date: 02/18/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	10:39am
AIR BLK	.00	10:40am
ACCY CHK	.08	10:40am
AIR BLK	.00	10:41am
SUB TEST	.00	10:42am
AIR BLK	.00	10:43am
SUB TEST	.00	10:44am
AIR BLK	.00	10:45am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593 Test Record Number: 1937
Test Date: 02/18/2022 Test Time: 10:46am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:46am
FLO	Pass	10:46am
FC	Pass	10:46am

Temperature Tests

Test	Status	Time
FC1	Pass	10:46am
SRC	Pass	10:46am
DET	Pass	10:46am
BAR	Pass	10:46am
BT	Pass	10:46am

Blank Tests

Test	Status	Time
AIR	Pass	10:47am


Printer Tests

Test	Status	Time
PRNT	Pass	10:47am

CRC Tests

Test	Status	Time
COMP	Pass	10:47am
CAL	Pass	10:47am

Preventive Maintenance
Status: Pass

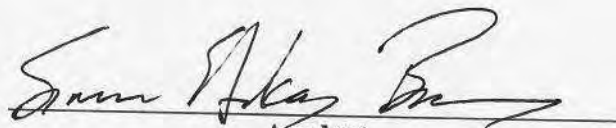
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Catawba Instrument Location Catawba Co SO
Instrument Serial No. 008687 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687
Test Date: 02/15/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	3:21pm
AIR BLK	.00	3:22pm
ACCY CHK	.08	3:23pm
AIR BLK	.00	3:24pm
SUB TEST	.00	3:24pm
AIR BLK	.00	3:25pm
SUB TEST	.00	3:27pm
AIR BLK	.00	3:28pm

Reported AC: .00 g/210L

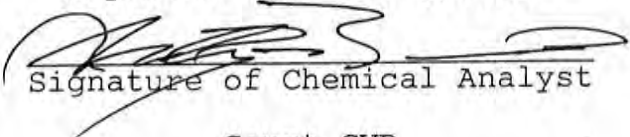
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687 Test Record Number: 3421
Test Date: 02/15/2022 Test Time: 3:28pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:28pm
FLO	Pass	3:28pm
FC	Pass	3:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:29pm
SRC	Pass	3:29pm
DET	Pass	3:29pm
BAR	Pass	3:29pm
BT	Pass	3:29pm

Blank Tests

Test	Status	Time
AIR	Pass	3:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:29pm

CRC Tests

Test	Status	Time
COMP	Pass	3:29pm
CAL	Pass	3:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Catawba Instrument Location Catawba Co SD
Instrument Serial No. 008821 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



George Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821
Test Date: 02/24/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	12:47pm
AIR BLK	.00	12:47pm
ACCY CHK	.07	12:48pm
AIR BLK	.00	12:49pm
SUB TEST	.00	12:50pm
AIR BLK	.00	12:50pm
SUB TEST	.00	12:52pm
AIR BLK	.00	12:53pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

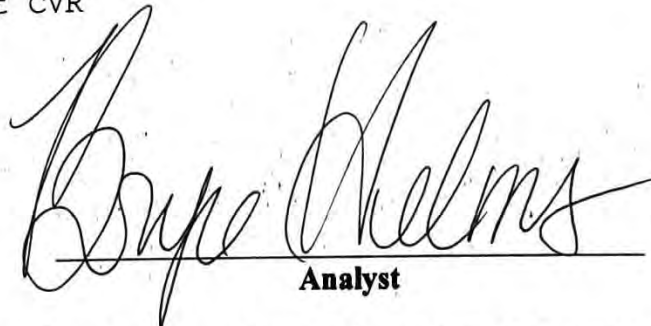
Analyst

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821 Test Record Number: 2250
Test Date: 02/24/2022 Test Time: 12:53pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:54pm
FLO	Pass	12:54pm
FC	Pass	12:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:54pm
SRC	Pass	12:54pm
DET	Pass	12:54pm
BAR	Pass	12:54pm
BT	Pass	12:54pm

Blank Tests

Test	Status	Time
AIR	Pass	12:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:54pm

CRC Tests

Test	Status	Time
COMP	Pass	12:55pm
CAL	Pass	12:55pm

Preventive Maintenance
Status: Pass

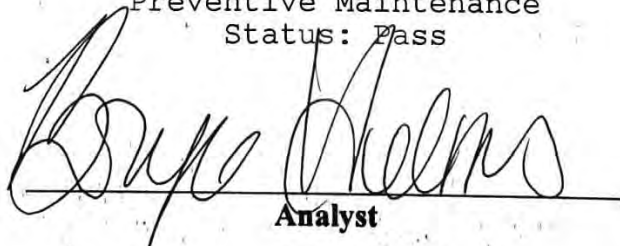
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Catawba Instrument Location Catawba Co SD
Instrument Serial No. 008821 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



George Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821
Test Date: 02/24/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	12:47pm
AIR BLK	.00	12:47pm
ACCY CHK	.07	12:48pm
AIR BLK	.00	12:49pm
SUB TEST	.00	12:50pm
AIR BLK	.00	12:50pm
SUB TEST	.00	12:52pm
AIR BLK	.00	12:53pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

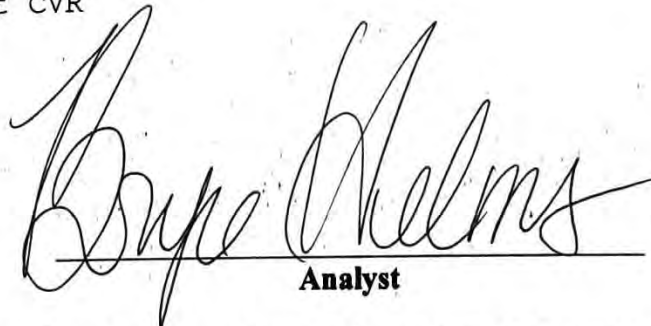

Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821 Test Record Number: 2250
Test Date: 02/24/2022 Test Time: 12:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:54pm
FLO	Pass	12:54pm
FC	Pass	12:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:54pm
SRC	Pass	12:54pm
DET	Pass	12:54pm
BAR	Pass	12:54pm
BT	Pass	12:54pm

Blank Tests

Test	Status	Time
AIR	Pass	12:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:54pm

CRC Tests

Test	Status	Time
COMP	Pass	12:55pm
CAL	Pass	12:55pm

Preventive Maintenance
Status: *Pass*

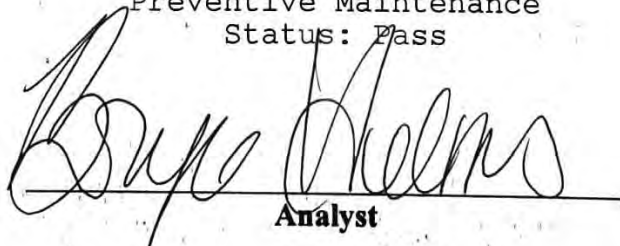

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Chowan Instrument Location Chowan Co Public Safety Center
Instrument Serial No. 008895 305 Freeman St, Edenton, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6043
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895
Test Date: 02/09/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	10:50am
AIR BLK	.00	10:50am
ACCY CHK	.07	10:51am
AIR BLK	.00	10:52am
SUB TEST	.00	10:53am
AIR BLK	.00	10:54am
SUB TEST	.00	10:55am
AIR BLK	.00	10:56am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895 Test Record Number: 1078
Test Date: 02/09/2022 Test Time: 10:57am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:57am
FLO	Pass	10:57am
FC	Pass	10:57am

Temperature Tests

Test	Status	Time
FC1	Pass	10:58am
SRC	Pass	10:58am
DET	Pass	10:58am
BAR	Pass	10:58am
BT	Pass	10:58am

Blank Tests

Test	Status	Time
AIR	Pass	10:58am

Printer Tests

Test	Status	Time
PRNT	Pass	10:58am

CRC Tests

Test	Status	Time
COMP	Pass	10:58am
CAL	Pass	10:58am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location Columbus County
Instrument Serial No. 008819 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008819
Test Date: 02/21/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	4:27pm
AIR BLK	.00	4:27pm
ACCY CHK	.08	4:28pm
AIR BLK	.00	4:29pm
SUB TEST	.00	4:30pm
AIR BLK	.00	4:31pm
SUB TEST	.00	4:32pm
AIR BLK	.00	4:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008819 Test Record Number: 848
Test Date: 02/21/2022 Test Time: 4:36pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	4:36pm
FLO	Pass	4:36pm
FC	Pass	4:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:36pm
SRC	Pass	4:36pm
DET	Pass	4:36pm
BAR	Pass	4:36pm
BT	Pass	4:36pm

Blank Tests

Test	Status	Time
AIR	Pass	4:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:37pm

CRC Tests

Test	Status	Time
COMP	Pass	4:37pm
CAL	Pass	4:37pm

Preventive Maintenance
Status: Pass

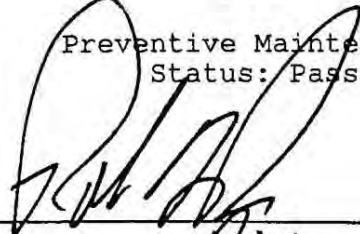

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location FT. Bragg

Instrument Serial No. 013868 L.E.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013868
Test Date: 02/23/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Garner, Joel K*
Permit Number: 0036-5156
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	10:46am
AIR BLK	.00	10:46am
ACCY CHK	.07	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:48am
AIR BLK	.00	10:49am
SUB TEST	.00	10:51am
AIR BLK	.00	10:52am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013868 Test Record Number: 218
Test Date: 02/23/2022 Test Time: 10:53am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:53am
FLO	Pass	10:53am
FC	Pass	10:53am

Temperature Tests

Test	Status	Time
FC1	Pass	10:53am
SRC	Pass	10:53am
DET	Pass	10:53am
BAR	Pass	10:53am
BT	Pass	10:53am

Blank Tests

Test	Status	Time
AIR	Pass	10:54am

Printer Tests

Test	Status	Time
PRNT	Pass	10:54am

CRC Tests

Test	Status	Time
COMP	Pass	10:54am
CAL	Pass	10:54am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cumberland Instrument Location FT Bragg
Instrument Serial No. 013870 L.E.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013870
Test Date: 02/23/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	10:43am
AIR BLK	.00	10:44am
ACCY CHK	.07	10:44am
AIR BLK	.00	10:46am
SUB TEST	.00	10:46am
AIR BLK	.00	10:47am
SUB TEST	.00	10:49am
AIR BLK	.00	10:49am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013870 Test Record Number: 282
Test Date: 02/23/2022 Test Time: 10:51am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:51am
FLO	Pass	10:51am
FC	Pass	10:51am

Temperature Tests

Test	Status	Time
FC1	Pass	10:51am
SRC	Pass	10:51am
DET	Pass	10:51am
BAR	Pass	10:51am
BT	Pass	10:51am

Blank Tests

Test	Status	Time
AIR	Pass	10:52am


Printer Tests

Test	Status	Time
PRNT	Pass	10:52am

CRC Tests

Test	Status	Time
COMP	Pass	10:52am
CAL	Pass	10:52am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Currituck Instrument Location Currituck Co. S.O. - Corolla

Instrument Serial No. 008949 1123 Ocean Trail, Corolla NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 1043 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CURRITUCK COUNTY SO-COROLLA 260

Serial Number: 008949

Test Date: 02/02/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	10:54am
AIR BLK	.00	10:54am
ACCY CHK	.08	10:55am
AIR BLK	.00	10:56am
SUB TEST	.00	10:57am
AIR BLK	.00	10:58am
SUB TEST	.00	10:59am
AIR BLK	.00	11:00am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY SO-COROLLA 260

Serial Number: 008949 Test Record Number: 635
Test Date: 02/02/2022 Test Time: 11:01am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:02am
FLO	Pass	11:02am
FC	Pass	11:02am

Temperature Tests

Test	Status	Time
FC1	Pass	11:02am
SRC	Pass	11:02am
DET	Pass	11:02am
BAR	Pass	11:02am
BT	Pass	11:02am

Blank Tests

Test	Status	Time
AIR	Pass	11:03am

Printer Tests

Test	Status	Time
PRNT	Pass	11:03am

CRC Tests

Test	Status	Time
COMP	Pass	11:03am
CAL	Pass	11:03am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dave Instrument Location Dave Co Detention Center

Instrument Serial No. 008588 1044 Driftwood Dr, Montez
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008588
Test Date: 02/03/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Guard, Kelly G
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	10:34am
AIR BLK	.00	10:35am
ACCY CHK	.08	10:35am
AIR BLK	.00	10:36am
SUB TEST	.00	10:37am
AIR BLK	.00	10:38am
SUB TEST	.00	10:39am
AIR BLK	.00	10:40am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008588 Test Record Number: 1120
Test Date: 02/03/2022 Test Time: 10:41am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:41am
FLO	Pass	10:41am
FC	Pass	10:41am

Temperature Tests

Test	Status	Time
FC1	Pass	10:41am
SRC	Pass	10:41am
DET	Pass	10:41am
BAR	Pass	10:41am
BT	Pass	10:41am

Blank Tests

Test	Status	Time
AIR	Pass	10:42am

Printer Tests

Test	Status	Time
PRNT	Pass	10:42am

CRC Tests

Test	Status	Time
COMP	Pass	10:42am
CAL	Pass	10:42am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dave Instrument Location Dave Co. Detention Center

Instrument Serial No. 008783 1044 Dr. Howard Dr., Mantoloking, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008783

Test Date: 02/28/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	12:10pm
AIR BLK	.00	12:10pm
ACCY CHK	.08	12:11pm
AIR BLK	.00	12:12pm
SUB TEST	.00	12:13pm
AIR BLK	.00	12:13pm
SUB TEST	.00	12:16pm
AIR BLK	.00	12:17pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008783 Test Record Number: 1086
Test Date: 02/28/2022 Test Time: 12:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:18pm
FLO	Pass	12:18pm
FC	Pass	12:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:18pm
SRC	Pass	12:18pm
DET	Pass	12:18pm
BAR	Pass	12:18pm
BT	Pass	12:18pm

Blank Tests

Test	Status	Time
AIR	Pass	12:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:19pm

CRC Tests

Test	Status	Time
COMP	Pass	12:19pm
CAL	Pass	12:19pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location Dare Co. Detention Center
Instrument Serial No. 108804 1044 Driftwood Dr, Manteo, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008804
Test Date: 02/03/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	10:12am
AIR BLK	.00	10:13am
ACCY CHK	.08	10:13am
AIR BLK	.00	10:15am
SUB TEST	.00	10:15am
AIR BLK	.00	10:16am
SUB TEST	.00	10:18am
AIR BLK	.00	10:19am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008804 Test Record Number: 2640
Test Date: 02/03/2022 Test Time: 10:19am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:20am
FLO	Pass	10:20am
FC	Pass	10:20am

Temperature Tests

Test	Status	Time
FC1	Pass	10:20am
SRC	Pass	10:20am
DET	Pass	10:20am
BAR	Pass	10:20am
BT	Pass	10:20am

Blank Tests

Test	Status	Time
AIR	Pass	10:21am

Printer Tests

Test	Status	Time
PRNT	Pass	10:21am

CRC Tests

Test	Status	Time
COMP	Pass	10:21am
CAL	Pass	10:21am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location Dare Co S.O. - Hatteras
Instrument Serial No. 008807 50347 Hwy NC 17, Buxton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO SO HATTERAS 270

Serial Number: 008807

Test Date: 02/01/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	10:14am
AIR BLK	.00	10:14am
ACCY CHK	.08	10:15am
AIR BLK	.00	10:16am
SUB TEST	.00	10:17am
AIR BLK	.00	10:18am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO SO HATTERAS 270

Serial Number: 008807 Test Record Number: 1261
Test Date: 02/01/2022 Test Time: 10:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:21am
FLO	Pass	10:21am
FC	Pass	10:21am

Temperature Tests

Test	Status	Time
FC1	Pass	10:21am
SRC	Pass	10:21am
DET	Pass	10:21am
BAR	Pass	10:21am
BT	Pass	10:21am

Blank Tests

Test	Status	Time
AIR	Pass	10:22am

Printer Tests

Test	Status	Time
PRNT	Pass	10:22am

CRC Tests

Test	Status	Time
COMP	Pass	10:22am
CAL	Pass	10:22am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIDSON Instrument Location DAVIDSON COUNTY JAIL

Instrument Serial No. 008845 LEXINGTON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY DAVIDSON CO JAIL 280

Serial Number: 008845
Test Date: 02/16/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118803

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	4:08pm
AIR BLK	.00	4:09pm
ACCY CHK	.08	4:10pm
AIR BLK	.00	4:11pm
SUB TEST	.00	4:12pm
AIR BLK	.00	4:13pm
SUB TEST	.00	4:14pm
AIR BLK	.00	4:15pm

Reported AC: .00 g/210L

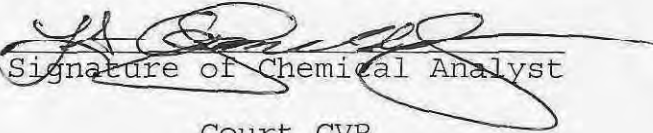
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY DAVIDSON CO JAIL 280

Serial Number: 008845 Test Record Number: 3739
Test Date: 02/16/2022 Test Time: 4:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:16pm
FLO	Pass	4:16pm
FC	Pass	4:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:17pm
SRC	Pass	4:17pm
DET	Pass	4:17pm
BAR	Pass	4:17pm
BT	Pass	4:17pm

Blank Tests

Test	Status	Time
AIR	Pass	4:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:17pm

CRC Tests

Test	Status	Time
COMP	Pass	4:17pm
CAL	Pass	4:17pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County DAVIDSON Instrument Location LEXINGTON POLICE

Instrument Serial No. 008883 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY LEXINGTON PD 280

Serial Number: 008883
Test Date: 02/15/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG131901

Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	3:48pm
AIR BLK	.00	3:49pm
ACCY CHK	.08	3:49pm
AIR BLK	.00	3:51pm
SUB TEST	.00	3:51pm
AIR BLK	.00	3:52pm
SUB TEST	.00	3:54pm
AIR BLK	.00	3:55pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY LEXINGTON PD 280

Serial Number: 008883 Test Record Number: 2416
Test Date: 02/15/2022 Test Time: 3:56pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:56pm
FLO	Pass	3:56pm
FC	Pass	3:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:56pm
SRC	Pass	3:56pm
DET	Pass	3:56pm
BAR	Pass	3:56pm
BT	Pass	3:56pm

Blank Tests

Test	Status	Time
AIR	Pass	3:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:57pm

CRC Tests

Test	Status	Time
COMP	Pass	3:57pm
CAL	Pass	3:57pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Durham Instrument Location Durham G Jail
Instrument Serial No. 1128859 219 S. Mangum St
Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859
Test Date: 02/03/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	1:25pm
AIR BLK	.00	1:25pm
ACCY CHK	.08	1:26pm
AIR BLK	.00	1:27pm
SUB TEST	.00	1:28pm
AIR BLK	.00	1:28pm
SUB TEST	.00	1:30pm
AIR BLK	.00	1:31pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859 Test Record Number: 2632
Test Date: 02/03/2022 Test Time: 1:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:32pm
FLO	Pass	1:32pm
FC	Pass	1:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:32pm
SRC	Pass	1:32pm
DET	Pass	1:32pm
BAR	Pass	1:32pm
BT	Pass	1:32pm

Blank Tests

Test	Status	Time
AIR	Pass	1:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:33pm

CRC Tests

Test	Status	Time
COMP	Pass	1:33pm
CAL	Pass	1:33pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DURHAM Instrument Location Durham Co Jail
Instrument Serial No. 608878 219 S Mangum St
Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 20 22 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. Bryant Signature of Certifying Official 671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878

Test Date: 02/03/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	1:15pm
AIR BLK	.00	1:16pm
ACCY CHK	.08	1:17pm
AIR BLK	.00	1:18pm
SUB TEST	.00	1:18pm
AIR BLK	.00	1:19pm
SUB TEST	.00	1:21pm
AIR BLK	.00	1:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878 Test Record Number: 5308
Test Date: 02/03/2022 Test Time: 1:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:26pm
FLO	Pass	1:26pm
FC	Pass	1:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:26pm
SRC	Pass	1:26pm
DET	Pass	1:26pm
BAR	Pass	1:26pm
BT	Pass	1:26pm

Blank Tests

Test	Status	Time
AIR	Pass	1:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:26pm

CRC Tests

Test	Status	Time
COMP	Pass	1:27pm
CAL	Pass	1:27pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Durham Instrument Location Durham Co. Jail
Instrument Serial No. 00891 219 S Mangum St
Durham NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



EAB Signature of Certifying Official 671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891

Test Date: 02/03/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	1:19pm
AIR BLK	.00	1:20pm
ACCY CHK	.08	1:21pm
AIR BLK	.00	1:22pm
SUB TEST	.00	1:22pm
AIR BLK	.00	1:23pm
SUB TEST	.00	1:25pm
AIR BLK	.00	1:26pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891 Test Record Number: 4522
Test Date: 02/03/2022 Test Time: 1:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:27pm
FLO	Pass	1:27pm
FC	Pass	1:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:27pm
SRC	Pass	1:27pm
DET	Pass	1:27pm
BAR	Pass	1:27pm
BT	Pass	1:27pm

Blank Tests

Test	Status	Time
AIR	Pass	1:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:28pm

CRC Tests

Test	Status	Time
COMP	Pass	1:28pm
CAL	Pass	1:28pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location Edgecombe Co. Magistrate's
Instrument Serial No. 008603 Office, 300 S. Anacosta Rd,
Tarboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008603
Test Date: 02/11/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	11:58am
AIR BLK	.00	11:58am
ACCY CHK	.08	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:01pm
AIR BLK	.00	12:02pm
SUB TEST	.00	12:03pm
AIR BLK	.00	12:04pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008603 Test Record Number: 2017
Test Date: 02/11/2022 Test Time: 12:05pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:06pm
FLO	Pass	12:06pm
FC	Pass	12:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:06pm
SRC	Pass	12:06pm
DET	Pass	12:06pm
BAR	Pass	12:06pm
BT	Pass	12:06pm

Blank Tests

Test	Status	Time
AIR	Pass	12:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:06pm

CRC Tests

Test	Status	Time
COMP	Pass	12:07pm
CAL	Pass	12:07pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Edgecombe Instrument Location Edgecombe Co. Magistrate's
Instrument Serial No. 008663 Office, 300 S. Anaronda Rd.,
Tarboro, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2027 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008663
Test Date: 02/11/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	12:13pm
AIR BLK	.00	12:14pm
ACCY CHK	.08	12:15pm
AIR BLK	.00	12:16pm
SUB TEST	.00	12:17pm
AIR BLK	.00	12:17pm
SUB TEST	.00	12:20pm
AIR BLK	.00	12:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008663 Test Record Number: 3447
Test Date: 02/11/2022 Test Time: 12:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:22pm
FLO	Pass	12:22pm
FC	Pass	12:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:22pm
SRC	Pass	12:22pm
DET	Pass	12:22pm
BAR	Pass	12:22pm
BT	Pass	12:22pm

Blank Tests

Test	Status	Time
AIR	Pass	12:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:23pm

CRC Tests

Test	Status	Time
COMP	Pass	12:23pm
CAL	Pass	12:23pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location FORSYTH CO. DETENTION

Instrument Serial No. 008583 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008583
Test Date: 02/07/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	9:47am
AIR BLK	.00	9:48am
ACCY CHK	.08	9:48am
AIR BLK	.00	9:49am
SUB TEST	.00	9:50am
AIR BLK	.00	9:51am
SUB TEST	.00	9:53am
AIR BLK	.00	9:53am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008583 Test Record Number: 8743
Test Date: 02/07/2022 Test Time: 9:54am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:55am
FLO	Pass	9:55am
FC	Pass	9:55am

Temperature Tests

Test	Status	Time
FC1	Pass	9:55am
SRC	Pass	9:55am
DET	Pass	9:55am
BAR	Pass	9:55am
BT	Pass	9:55am

Blank Tests

Test	Status	Time
AIR	Pass	9:56am

Printer Tests

Test	Status	Time
PRNT	Pass	9:56am

CRC Tests

Test	Status	Time
COMP	Pass	9:56am
CAL	Pass	9:56am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH CO. DETENTION

Instrument Serial No. 008659 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008659
Test Date: 02/07/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	9:51am
AIR BLK	.00	9:52am
ACCY CHK	.07	9:52am
AIR BLK	.00	9:54am
SUB TEST	.00	9:55am
AIR BLK	.00	9:56am
SUB TEST	.00	9:57am
AIR BLK	.00	9:58am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008659 Test Record Number: 5849
Test Date: 02/07/2022 Test Time: 10:00am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:00am
FLO	Pass	10:00am
FC	Pass	10:00am

Temperature Tests

Test	Status	Time
FC1	Pass	10:00am
SRC	Pass	10:00am
DET	Pass	10:00am
BAR	Pass	10:00am
BT	Pass	10:00am

Blank Tests

Test	Status	Time
AIR	Pass	10:01am


Printer Tests

Test	Status	Time
PRNT	Pass	10:01am

CRC Tests

Test	Status	Time
COMP	Pass	10:01am
CAL	Pass	10:01am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH CO. DETENTION
Instrument Serial No. 008925 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008925
Test Date: 02/07/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG118803
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	9:56am
AIR BLK	.00	9:57am
ACCY CHK	.08	9:58am
AIR BLK	.00	9:59am
SUB TEST	.00	10:01am
AIR BLK	.00	10:02am
SUB TEST	.00	10:04am
AIR BLK	.00	10:05am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008925 Test Record Number: 4097
Test Date: 02/07/2022 Test Time: 10:06am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:07am
FLO	Pass	10:07am
FC	Pass	10:07am

Temperature Tests

Test	Status	Time
FC1	Pass	10:07am
SRC	Pass	10:07am
DET	Pass	10:07am
BAR	Pass	10:07am
BT	Pass	10:07am

Blank Tests

Test	Status	Time
AIR	Pass	10:08am


Printer Tests

Test	Status	Time
PRNT	Pass	10:08am

CRC Tests

Test	Status	Time
COMP	Pass	10:08am
CAL	Pass	10:08am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Gaston County 80
Instrument Serial No. 008910 Gaston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008910
Test Date: 02/10/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	1:12pm
AIR BLK	.00	1:12pm
ACCY CHK	.08	1:13pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:15pm
AIR BLK	.00	1:15pm
SUB TEST	.00	1:17pm
AIR BLK	.00	1:18pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008910 Test Record Number: 1263
Test Date: 02/10/2022 Test Time: 1:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:19pm
FLO	Pass	1:19pm
FC	Pass	1:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:19pm
SRC	Pass	1:19pm
DET	Pass	1:19pm
BAR	Pass	1:19pm
BT	Pass	1:19pm

Blank Tests

Test	Status	Time
AIR	Pass	1:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:19pm

CRC Tests

Test	Status	Time
COMP	Pass	1:20pm
CAL	Pass	1:20pm

Preventive Maintenance
Status: *Pass*

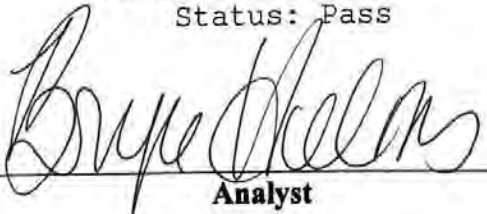

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Greene Instrument Location Greene Co S.O.

Instrument Serial No. 008670 301 W. Greene St, Snow Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GREENE COUNTY GREENE CO SO 390

Serial Number: 008670

Test Date: 02/08/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	10:55am
AIR BLK	.00	10:55am
ACCY CHK	.08	10:56am
AIR BLK	.00	10:57am
SUB TEST	.00	10:58am
AIR BLK	.00	10:59am
SUB TEST	.00	11:00am
AIR BLK	.00	11:01am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GREENE COUNTY GREENE CO SO 390

Serial Number: 008670 Test Record Number: 2198
Test Date: 02/08/2022 Test Time: 11:02am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:02am
FLO	Pass	11:02am
FC	Pass	11:02am

Temperature Tests

Test	Status	Time
FC1	Pass	11:02am
SRC	Pass	11:02am
DET	Pass	11:02am
BAR	Pass	11:02am
BT	Pass	11:02am

Blank Tests

Test	Status	Time
AIR	Pass	11:03am


Printer Tests

Test	Status	Time
PRNT	Pass	11:03am

CRC Tests

Test	Status	Time
COMP	Pass	11:03am
CAL	Pass	11:03am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County GUILFORD Instrument Location GREENSBORO JAIL
Instrument Serial No. 008638 GREENSBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008638
Test Date: 02/14/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118803

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	12:21pm
AIR BLK	.00	12:22pm
ACCY CHK	.08	12:23pm
AIR BLK	.00	12:24pm
SUB TEST	.00	12:25pm
AIR BLK	.00	12:25pm
SUB TEST	.00	12:27pm
AIR BLK	.00	12:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY, GREENSBORO JAIL 400

Serial Number: 008638 Test Record Number: 5197
Test Date: 02/14/2022 Test Time: 12:30pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:30pm
FLO	Pass	12:30pm
FC	Pass	12:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:30pm
SRC	Pass	12:30pm
DET	Pass	12:30pm
BAR	Pass	12:30pm
BT	Pass	12:30pm

Blank Tests

Test	Status	Time
AIR	Pass	12:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:31pm

CRC Tests

Test	Status	Time
COMP	Pass	12:31pm
CAL	Pass	12:31pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County GUILFORD Instrument Location GREENSBORO JAIL

Instrument Serial No. 008790 GREENSBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 669 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008790

Test Date: 02/14/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118803

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	12:50pm
AIR BLK	.00	12:51pm
ACCY CHK	.08	12:52pm
AIR BLK	.00	12:53pm
SUB TEST	.00	12:54pm
AIR BLK	.00	12:55pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:57pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008790 Test Record Number: 7555
Test Date: 02/14/2022 Test Time: 12:58pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:58pm
FLO	Pass	12:58pm
FC	Pass	12:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:59pm
SRC	Pass	12:59pm
DET	Pass	12:59pm
BAR	Pass	12:59pm
BT	Pass	12:59pm

Blank Tests

Test	Status	Time
AIR	Pass	12:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:59pm

CRC Tests

Test	Status	Time
COMP	Pass	1:00pm
CAL	Pass	1:00pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County GUILFORD Instrument Location GREENSBORO JAIL

Instrument Serial No. 008794 GREENSBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008794
Test Date: 02/14/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118803

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	12:20pm
AIR BLK	.00	12:21pm
ACCY CHK	.07	12:22pm
AIR BLK	.00	12:23pm
SUB TEST	.00	12:23pm
AIR BLK	.00	12:24pm
SUB TEST	.00	12:26pm
AIR BLK	.00	12:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008794 Test Record Number: 7557
Test Date: 02/14/2022 Test Time: 12:28pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:28pm
FLO	Pass	12:28pm
FC	Pass	12:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:29pm
SRC	Pass	12:29pm
DET	Pass	12:29pm
BAR	Pass	12:29pm
BT	Pass	12:29pm

Blank Tests

Test	Status	Time
AIR	Pass	12:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:29pm

CRC Tests

Test	Status	Time
COMP	Pass	12:29pm
CAL	Pass	12:29pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Habitat Instrument Location Foamoke Rapids PD

Instrument Serial No. 008656 1040 Foamoke Ave
Foamoke Rapids, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. Smith Signature of Certifying Official 671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: 008656
Test Date: 02/28/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022


Test	g/210L	Time
DIAG	Pass	5:31pm
AIR BLK	.00	5:31pm
ACCY CHK	.07	5:32pm
AIR BLK	.00	5:33pm
SUB TEST	.00	5:34pm
AIR BLK	.00	5:35pm
SUB TEST	.00	5:36pm
AIR BLK	.00	5:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

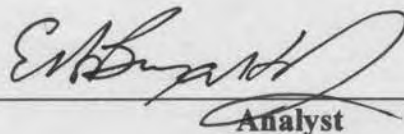

Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: 008656 Test Record Number: 816
Test Date: 02/28/2022 Test Time: 5:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:40pm
FLO	Pass	5:40pm
FC	Pass	5:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:40pm
SRC	Pass	5:40pm
DET	Pass	5:40pm
BAR	Pass	5:40pm
BT	Pass	5:40pm

Blank Tests

Test	Status	Time
AIR	Pass	5:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:41pm

CRC Tests

Test	Status	Time
COMP	Pass	5:41pm
CAL	Pass	5:41pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Halifax Instrument Location Halifax Co. S.O.
Instrument Serial No. 008695 335 Ferrell Lane
Halifax, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. Bryant
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695
Test Date: 02/22/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	6:00pm
AIR BLK	.00	6:00pm
ACCY CHK	.08	6:01pm
AIR BLK	.00	6:02pm
SUB TEST	.00	6:03pm
AIR BLK	.00	6:03pm
SUB TEST	.00	6:05pm
AIR BLK	.00	6:06pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695 Test Record Number: 3325
Test Date: 02/22/2022 Test Time: 6:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:08pm
FLO	Pass	6:08pm
FC	Pass	6:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:09pm
SRC	Pass	6:09pm
DET	Pass	6:09pm
BAR	Pass	6:09pm
BT	Pass	6:09pm

Blank Tests

Test	Status	Time
AIR	Pass	6:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:09pm

CRC Tests

Test	Status	Time
COMP	Pass	6:09pm
CAL	Pass	6:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Harnett Instrument Location Dunn Police
Instrument Serial No. 008644 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DUNN PD 420

Serial Number: 008644
Test Date: 02/01/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	10:05am
AIR BLK	.00	10:05am
ACCY CHK	.07	10:06am
AIR BLK	.00	10:07am
SUB TEST	.00	10:08am
AIR BLK	.00	10:09am
SUB TEST	.00	10:10am
AIR BLK	.00	10:11am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DUNN PD 420

Serial Number: 008644 Test Record Number: 1545
Test Date: 02/01/2022 Test Time: 10:12am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:12am
FLO	Pass	10:12am
FC	Pass	10:12am

Temperature Tests

Test	Status	Time
FC1	Pass	10:12am
SRC	Pass	10:12am
DET	Pass	10:12am
BAR	Pass	10:12am
BT	Pass	10:12am

Blank Tests

Test	Status	Time
AIR	Pass	10:13am


Printer Tests

Test	Status	Time
PRNT	Pass	10:13am

CRC Tests

Test	Status	Time
COMP	Pass	10:13am
CAL	Pass	10:13am

Preventive Maintenance
Status: Pass

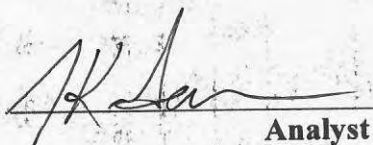

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County HARNETT Instrument Location HARNETT CO.
Instrument Serial No. 008729 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1ST day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008729
Test Date: 02/01/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	9:51am
AIR BLK	.00	9:52am
ACCY CHK	.07	9:53am
AIR BLK	.00	9:54am
SUB TEST	.00	9:55am
AIR BLK	.00	9:56am
SUB TEST	.00	9:57am
AIR BLK	.00	9:58am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008729 Test Record Number: 2537
Test Date: 02/01/2022 Test Time: 9:59am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:00am
FLO	Pass	10:00am
FC	Pass	10:00am

Temperature Tests

Test	Status	Time
FC1	Pass	10:00am
SRC	Pass	10:00am
DET	Pass	10:00am
BAR	Pass	10:00am
BT	Pass	10:00am

Blank Tests

Test	Status	Time
AIR	Pass	10:00am


Printer Tests

Test	Status	Time
PRNT	Pass	10:01am

CRC Tests

Test	Status	Time
COMP	Pass	10:01am
CAL	Pass	10:01am

Preventive Maintenance
Status: Pass

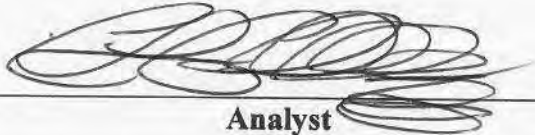

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County HARNETT Instrument Location HARNETT Co.
Instrument Serial No. 008730 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1ST day of FEBRUARY, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008730
Test Date: 02/01/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	10:05am
AIR BLK	.00	10:05am
ACCY CHK	.08	10:06am
AIR BLK	.00	10:07am
SUB TEST	.00	10:07am
AIR BLK	.00	10:08am
SUB TEST	.00	10:10am
AIR BLK	.00	10:11am

Reported AC: .00 g/210L

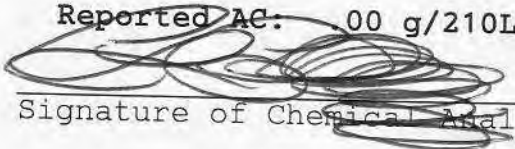
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008730 Test Record Number: 3976
Test Date: 02/01/2022 Test Time: 10:12am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:12am
FLO	Pass	10:12am
FC	Pass	10:12am

Temperature Tests

Test	Status	Time
FC1	Pass	10:12am
SRC	Pass	10:12am
DET	Pass	10:12am
BAR	Pass	10:12am
BT	Pass	10:12am

Blank Tests

Test	Status	Time
AIR	Pass	10:13am

Printer Tests

Test	Status	Time
PRNT	Pass	10:13am

CRC Tests

Test	Status	Time
COMP	Pass	10:13am
CAL	Pass	10:13am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Henderson Instrument Location Henderson County Detention

Instrument Serial No. 0087116 Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 6089 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HENDERSON COUNTY HENDERSON COUNTY
DETENTION 440

Serial Number: 008916
Test Date: 02/23/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	2:47pm
AIR BLK	.00	2:47pm
ACCY CHK	.08	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm
SUB TEST	.00	2:52pm
AIR BLK	.00	2:53pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HENDERSON COUNTY HENDERSON COUNTY DETENTION 440

Serial Number: 008916 Test Record Number: 1568
Test Date: 02/23/2022 Test Time: 2:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:54pm
FLO	Pass	2:54pm
FC	Pass	2:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:54pm
SRC	Pass	2:54pm
DET	Pass	2:54pm
BAR	Pass	2:54pm
BT	Pass	2:54pm

Blank Tests

Test	Status	Time
AIR	Pass	2:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:55pm

CRC Tests

Test	Status	Time
COMP	Pass	2:55pm
CAL	Pass	2:55pm

Preventive Maintenance
Status: Pass

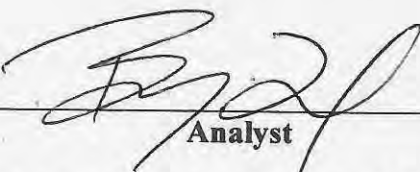

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hertford Instrument Location Ahoskie PD

Instrument Serial No. 008848 705 W. Main St, Ahoskie, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kur Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848

Test Date: 02/07/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	9:59am
AIR BLK	.00	10:00am
ACCY CHK	.07	10:00am
AIR BLK	.00	10:02am
SUB TEST	.00	10:02am
AIR BLK	.00	10:03am
SUB TEST	.00	10:05am
AIR BLK	.00	10:06am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848 Test Record Number: 1673
Test Date: 02/07/2022 Test Time: 10:06am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:07am
FLO	Pass	10:07am
FC	Pass	10:07am

Temperature Tests

Test	Status	Time
FC1	Pass	10:07am
SRC	Pass	10:07am
DET	Pass	10:07am
BAR	Pass	10:07am
BT	Pass	10:07am

Blank Tests

Test	Status	Time
AIR	Pass	10:08am


Printer Tests

Test	Status	Time
PRNT	Pass	10:08am

CRC Tests

Test	Status	Time
COMP	Pass	10:08am
CAL	Pass	10:08am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hertford Instrument Location Murfreeboro PD

Instrument Serial No. 008906 115 E. Broad St. Murfreeboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906
Test Date: 02/07/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023


Test	g/210L	Time
DIAG	Pass	12:18pm
AIR BLK	.00	12:18pm
ACCY CHK	.08	12:19pm
AIR BLK	.00	12:20pm
SUB TEST	.00	12:21pm
AIR BLK	.00	12:22pm
SUB TEST	.00	12:24pm
AIR BLK	.00	12:24pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906 Test Record Number: 835
Test Date: 02/07/2022 Test Time: 12:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:25pm
FLO	Pass	12:25pm
FC	Pass	12:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:26pm
SRC	Pass	12:26pm
DET	Pass	12:26pm
BAR	Pass	12:26pm
BT	Pass	12:26pm

Blank Tests

Test	Status	Time
AIR	Pass	12:26pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:26pm

CRC Tests

Test	Status	Time
COMP	Pass	12:27pm
CAL	Pass	12:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hyde Instrument Location Hyde Co. S.D. - Occoake
Instrument Serial No. 008797 NC 12, Occoake NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

043
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO OCRACOKE 470

Serial Number: 008797
Test Date: 02/01/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	1:57pm
AIR BLK	.00	1:58pm
ACCY CHK	.08	1:59pm
AIR BLK	.00	2:00pm
SUB TEST	.00	2:00pm
AIR BLK	.00	2:01pm
SUB TEST	.00	2:03pm
AIR BLK	.00	2:04pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO OCRACOKE 470

Serial Number: 008797 Test Record Number: 634
Test Date: 02/01/2022 Test Time: 2:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:06pm
FLO	Pass	2:06pm
FC	Pass	2:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:07pm
SRC	Pass	2:07pm
DET	Pass	2:07pm
BAR	Pass	2:07pm
BT	Pass	2:07pm

Blank Tests

Test	Status	Time
AIR	Pass	2:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:07pm

CRC Tests

Test	Status	Time
COMP	Pass	2:07pm
CAL	Pass	2:07pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hyde Instrument Location Hyde Co. S.D.
Instrument Serial No. 004801 1233 Main St, S. Hyde, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801

Test Date: 02/10/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	10:16am
AIR BLK	.00	10:17am
ACCY CHK	.07	10:17am
AIR BLK	.00	10:18am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am
SUB TEST	.00	10:22am
AIR BLK	.00	10:22am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801 Test Record Number: 633
Test Date: 02/10/2022 Test Time: 10:24am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:24am
FLO	Pass	10:24am
FC	Pass	10:24am

Temperature Tests

Test	Status	Time
FC1	Pass	10:24am
SRC	Pass	10:24am
DET	Pass	10:24am
BAR	Pass	10:24am
BT	Pass	10:24am

Blank Tests

Test	Status	Time
AIR	Pass	10:25am


Printer Tests

Test	Status	Time
PRNT	Pass	10:25am

CRC Tests

Test	Status	Time
COMP	Pass	10:25am
CAL	Pass	10:25am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Tredell Instrument Location Mooreville PD
Instrument Serial No. 008685 Mooreville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685

Test Date: 02/07/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	11:53am
AIR BLK	.00	11:54am
ACCY CHK	.08	11:55am
AIR BLK	.00	11:56am
SUB TEST	.00	11:57am
AIR BLK	.00	11:57am
SUB TEST	.00	11:59am
AIR BLK	.00	12:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685 Test Record Number: 3867
Test Date: 02/07/2022 Test Time: 12:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:01pm
FLO	Pass	12:01pm
FC	Pass	12:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:01pm
SRC	Pass	12:01pm
DET	Pass	12:01pm
BAR	Pass	12:01pm
BT	Pass	12:01pm

Blank Tests

Test	Status	Time
AIR	Pass	12:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:02pm

CRC Tests

Test	Status	Time
COMP	Pass	12:02pm
CAL	Pass	12:02pm

Preventive Maintenance
Status: *Pass*

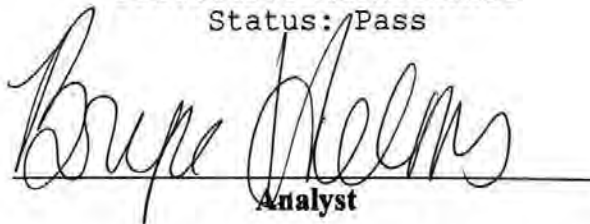
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Lenoir Instrument Location Kinston P.D.
Instrument Serial No. 008624 205 E. King St. Kinston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY KINSTON PD 530

Serial Number: 008624
Test Date: 02/08/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Guard, Kelly G
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118805
Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	1:06pm
AIR BLK	.00	1:07pm
ACCY CHK	.08	1:08pm
AIR BLK	.00	1:09pm
SUB TEST	.00	1:10pm
AIR BLK	.00	1:10pm
SUB TEST	.00	1:12pm
AIR BLK	.00	1:13pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

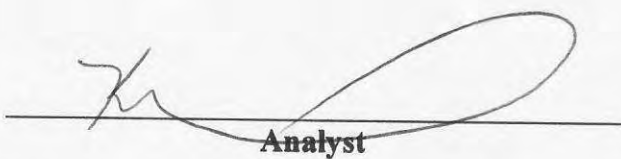

Analyst

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY KINSTON PD 530

Serial Number: 008624 Test Record Number: 1992
Test Date: 02/08/2022 Test Time: 1:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:14pm
FLO	Pass	1:14pm
FC	Pass	1:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:14pm
SRC	Pass	1:14pm
DET	Pass	1:14pm
BAR	Pass	1:14pm
BT	Pass	1:14pm

Blank Tests

Test	Status	Time
AIR	Pass	1:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:15pm

CRC Tests

Test	Status	Time
COMP	Pass	1:15pm
CAL	Pass	1:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Lenoir Instrument Location Lenoir Co S.O.

Instrument Serial No. 008639 130 Queen St., Kinston, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008639

Test Date: 02/08/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	1:44pm
AIR BLK	.00	1:45pm
ACCY CHK	.08	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:47pm
AIR BLK	.00	1:48pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008639 Test Record Number: 3607
Test Date: 02/08/2022 Test Time: 1:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:52pm
FLO	Pass	1:52pm
FC	Pass	1:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:53pm
SRC	Pass	1:53pm
DET	Pass	1:53pm
BAR	Pass	1:53pm
BT	Pass	1:53pm

Blank Tests

Test	Status	Time
AIR	Pass	1:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:53pm

CRC Tests

Test	Status	Time
COMP	Pass	1:53pm
CAL	Pass	1:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Lincoln Instrument Location Lincoln Co SO
Instrument Serial No. 008683 Lincolnton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008683
Test Date: 02/15/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	4:34pm
AIR BLK	.00	4:35pm
ACCY CHK	.08	4:36pm
AIR BLK	.00	4:37pm
SUB TEST	.00	4:38pm
AIR BLK	.00	4:39pm
SUB TEST	.00	4:40pm
AIR BLK	.00	4:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008683 Test Record Number: 980
Test Date: 02/15/2022 Test Time: 4:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:42pm
FLO	Pass	4:42pm
FC	Pass	4:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:42pm
SRC	Pass	4:42pm
DET	Pass	4:42pm
BAR	Pass	4:42pm
BT	Pass	4:42pm

Blank Tests

Test	Status	Time
AIR	Pass	4:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:43pm

CRC Tests

Test	Status	Time
COMP	Pass	4:43pm
CAL	Pass	4:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location Lincoln Co Courthouse
Instrument Serial No. 008823 Lincolnton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY COURTHOUSE 540

Serial Number: 008823
Test Date: 02/10/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107502

Exp Date: 03/16/2023


Test	g/210L	Time
DIAG	Pass	11:28am
AIR BLK	.00	11:29am
ACCY CHK	.08	11:29am
AIR BLK	.00	11:30am
SUB TEST	.00	11:31am
AIR BLK	.00	11:32am
SUB TEST	.00	11:33am
AIR BLK	.00	11:34am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

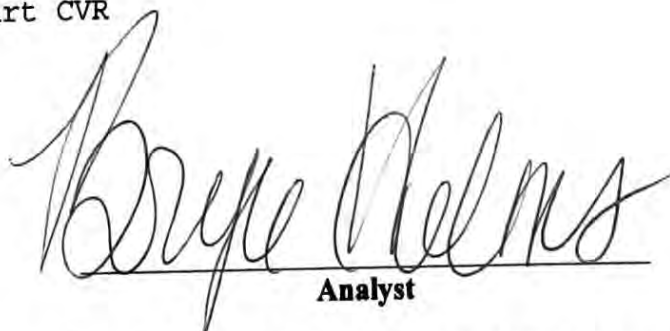

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY COURTHOUSE 540

Serial Number: 008823 Test Record Number: 1736
Test Date: 02/10/2022 Test Time: 11:34am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:35am
FLO	Pass	11:35am
FC	Pass	11:35am

Temperature Tests

Test	Status	Time
FC1	Pass	11:35am
SRC	Pass	11:35am
DET	Pass	11:35am
BAR	Pass	11:35am
BT	Pass	11:35am

Blank Tests

Test	Status	Time
AIR	Pass	11:36am


Printer Tests

Test	Status	Time
PRNT	Pass	11:36am

CRC Tests

Test	Status	Time
COMP	Pass	11:36am
CAL	Pass	11:36am

Preventive Maintenance
Status: Pass

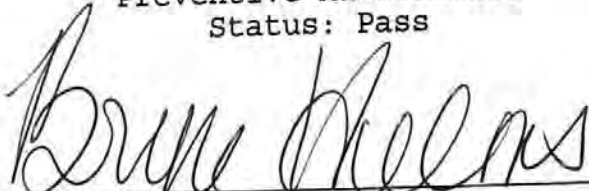

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location Lincoln County Jail
Instrument Serial No. 008827 Lincolnton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827
Test Date: 02/10/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	12:04pm
AIR BLK	.00	12:05pm
ACCY CHK	.07	12:06pm
AIR BLK	.00	12:07pm
SUB TEST	.00	12:07pm
AIR BLK	.00	12:08pm
SUB TEST	.00	12:10pm
AIR BLK	.00	12:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

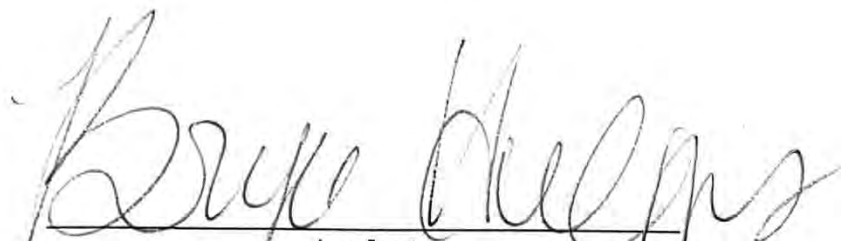
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827 Test Record Number: 3709
Test Date: 02/10/2022 Test Time: 12:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:11pm
FLO	Pass	12:11pm
FC	Pass	12:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:11pm
SRC	Pass	12:11pm
DET	Pass	12:11pm
BAR	Pass	12:11pm
BT	Pass	12:11pm

Blank Tests

Test	Status	Time
AIR	Pass	12:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:12pm

CRC Tests

Test	Status	Time
COMP	Pass	12:12pm
CAL	Pass	12:12pm

Preventive Maintenance
Status: *Pass*

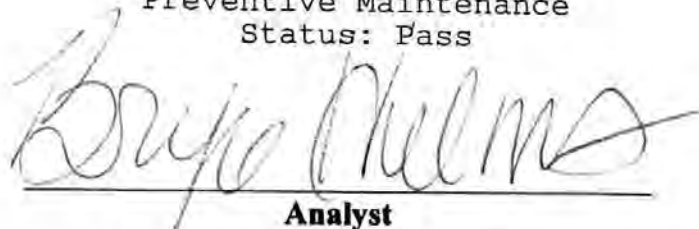

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location Lincoln County Jail
Instrument Serial No. 008827 Lincolnton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827
Test Date: 02/10/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	12:04pm
AIR BLK	.00	12:05pm
ACCY CHK	.07	12:06pm
AIR BLK	.00	12:07pm
SUB TEST	.00	12:07pm
AIR BLK	.00	12:08pm
SUB TEST	.00	12:10pm
AIR BLK	.00	12:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827 Test Record Number: 3709
Test Date: 02/10/2022 Test Time: 12:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:11pm
FLO	Pass	12:11pm
FC	Pass	12:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:11pm
SRC	Pass	12:11pm
DET	Pass	12:11pm
BAR	Pass	12:11pm
BT	Pass	12:11pm

Blank Tests

Test	Status	Time
AIR	Pass	12:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:12pm

CRC Tests

Test	Status	Time
COMP	Pass	12:12pm
CAL	Pass	12:12pm

Preventive Maintenance
Status: *Pass*

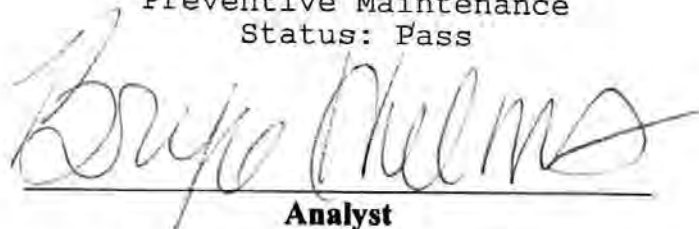

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Madison Instrument Location Madison County Jail
Instrument Serial No. 008599 Marshall, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

60698
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: 008599

Test Date: 02/03/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	10:14am
AIR BLK	.00	10:15am
ACCY CHK	.08	10:16am
AIR BLK	.00	10:17am
SUB TEST	.00	10:17am
AIR BLK	.00	10:18am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am

Reported AC: .00 g/210L

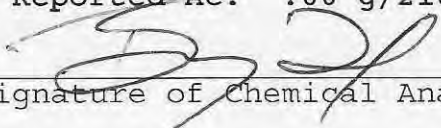
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: 008599 Test Record Number: 1243
Test Date: 02/03/2022 Test Time: 10:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:21am
FLO	Pass	10:21am
FC	Pass	10:21am

Temperature Tests

Test	Status	Time
FC1	Pass	10:21am
SRC	Pass	10:21am
DET	Pass	10:21am
BAR	Pass	10:21am
BT	Pass	10:21am

Blank Tests

Test	Status	Time
AIR	Pass	10:22am

Printer Tests

Test	Status	Time
PRNT	Pass	10:22am

CRC Tests

Test	Status	Time
COMP	Pass	10:22am
CAL	Pass	10:22am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County McDowell Instrument Location McDowell County Jail
Instrument Serial No. 008983 Maxon, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6608
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008888
Test Date: 02/01/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022


Test	g/210L	Time
DIAG	Pass	11:44am
AIR BLK	.00	11:44am
ACCY CHK	.07	11:45am
AIR BLK	.00	11:46am
SUB TEST	.00	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:50am
AIR BLK	.00	11:51am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

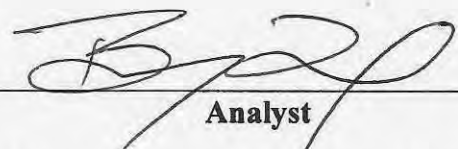

Analyst

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008888 Test Record Number: 1624
Test Date: 02/01/2022 Test Time: 11:51am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:51am
FLO	Pass	11:51am
FC	Pass	11:51am

Temperature Tests

Test	Status	Time
FC1	Pass	11:51am
SRC	Pass	11:51am
DET	Pass	11:51am
BAR	Pass	11:51am
BT	Pass	11:51am

Blank Tests

Test	Status	Time
AIR	Pass	11:52am


Printer Tests

Test	Status	Time
PRNT	Pass	11:52am

CRC Tests

Test	Status	Time
COMP	Pass	11:52am
CAL	Pass	11:52am

Preventive Maintenance
Status: Pass

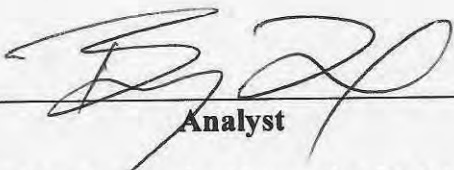

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County McDowell Instrument Location McDowell County Jail

Instrument Serial No. 005892 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6068
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008892

Test Date: 02/01/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132001

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	11:50am
AIR BLK	.00	11:50am
ACCY CHK	.08	11:51am
AIR BLK	.00	11:52am
SUB TEST	.00	11:52am
AIR BLK	.00	11:53am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am

Reported AC: .00 g/210L

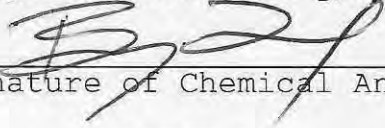

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008892 Test Record Number: 1067
Test Date: 02/01/2022 Test Time: 11:56am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:56am
FLO	Pass	11:56am
FC	Pass	11:56am

Temperature Tests

Test	Status	Time
FC1	Pass	11:57am
SRC	Pass	11:57am
DET	Pass	11:57am
BAR	Pass	11:57am
BT	Pass	11:57am

Blank Tests

Test	Status	Time
AIR	Pass	11:57am

Printer Tests

Test	Status	Time
PRNT	Pass	11:57am

CRC Tests

Test	Status	Time
COMP	Pass	11:57am
CAL	Pass	11:57am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location CMPD LEC
Instrument Serial No. 008691 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boye Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691

Test Date: 02/15/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	12:18pm
AIR BLK	.00	12:19pm
ACCY CHK	.08	12:19pm
AIR BLK	.00	12:20pm
SUB TEST	.00	12:20pm
AIR BLK	.00	12:21pm
SUB TEST	.00	12:23pm
AIR BLK	.00	12:24pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691 Test Record Number: 8676
Test Date: 02/15/2022 Test Time: 12:24pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:24pm
FLO	Pass	12:24pm
FC	Pass	12:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:25pm
SRC	Pass	12:25pm
DET	Pass	12:25pm
BAR	Pass	12:25pm
BT	Pass	12:25pm

Blank Tests

Test	Status	Time
AIR	Pass	12:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:25pm

CRC Tests

Test	Status	Time
COMP	Pass	12:25pm
CAL	Pass	12:25pm

Preventive Maintenance
Status: *Pass*

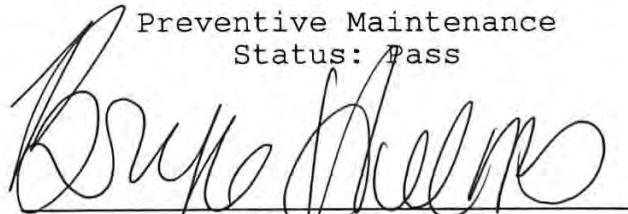

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Cornelius PD
Instrument Serial No. 0082692 Cornelius, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692
Test Date: 02/03/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118804


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	4:28pm
AIR BLK	.00	4:28pm
ACCY CHK	.08	4:29pm
AIR BLK	.00	4:30pm
SUB TEST	.00	4:31pm
AIR BLK	.00	4:32pm
SUB TEST	.00	4:33pm
AIR BLK	.00	4:34pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692 Test Record Number: 3204
Test Date: 02/03/2022 Test Time: 4:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:35pm
FLO	Pass	4:35pm
FC	Pass	4:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:35pm
SRC	Pass	4:35pm
DET	Pass	4:35pm
BAR	Pass	4:35pm
BT	Pass	4:35pm

Blank Tests

Test	Status	Time
AIR	Pass	4:36pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:36pm

CRC Tests

Test	Status	Time
COMP	Pass	4:36pm
CAL	Pass	4:36pm

Preventive Maintenance
Status: *Pass*

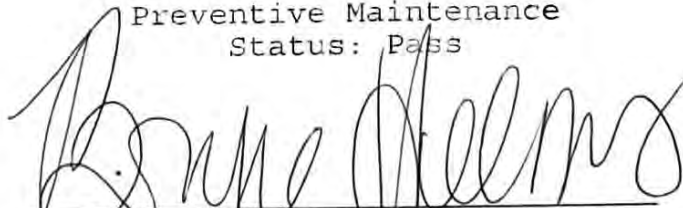

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Matthews PD
Instrument Serial No. 0086999 Matthews, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699
Test Date: 02/08/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	12:57pm
AIR BLK	.00	12:58pm
ACCY CHK	.07	12:59pm
AIR BLK	.00	1:00pm
SUB TEST	.00	1:01pm
AIR BLK	.00	1:02pm
SUB TEST	.00	1:03pm
AIR BLK	.00	1:04pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699 Test Record Number: 2965
Test Date: 02/08/2022 Test Time: 1:04pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:05pm
FLO	Pass	1:05pm
FC	Pass	1:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:05pm
SRC	Pass	1:05pm
DET	Pass	1:05pm
BAR	Pass	1:05pm
BT	Pass	1:05pm

Blank Tests

Test	Status	Time
AIR	Pass	1:06pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:06pm

CRC Tests

Test	Status	Time
COMP	Pass	1:06pm
CAL	Pass	1:06pm

Preventive Maintenance
Status: *Pass*

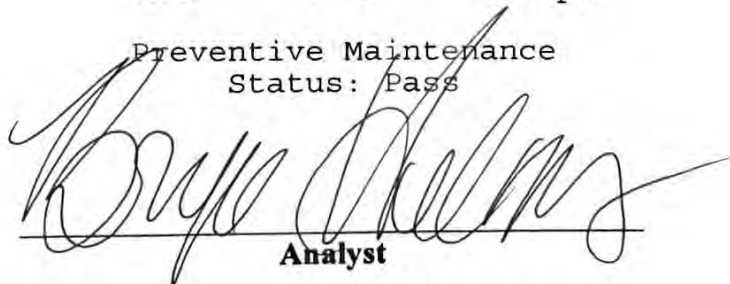

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Pineville Police Department
Instrument Serial No. 008703 Pineville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703
Test Date: 02/02/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001


Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	3:40pm
AIR BLK	.00	3:40pm
ACCY CHK	.08	3:41pm
AIR BLK	.00	3:42pm
SUB TEST	.00	3:43pm
AIR BLK	.00	3:44pm
SUB TEST	.00	3:45pm
AIR BLK	.00	3:46pm

Reported AQ: .00 g/210L


Signature of Chemical Analyst

Court CVR

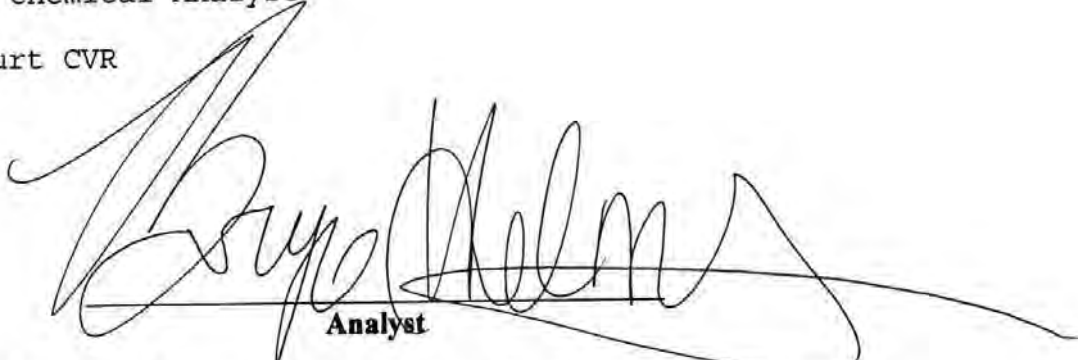
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703 Test Record Number: 6053
Test Date: 02/02/2022 Test Time: 3:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:47pm
FLO	Pass	3:47pm
FC	Pass	3:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:47pm
SRC	Pass	3:47pm
DET	Pass	3:47pm
BAR	Pass	3:47pm
BT	Pass	3:47pm

Blank Tests

Test	Status	Time
AIR	Pass	3:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:48pm

CRC Tests

Test	Status	Time
COMP	Pass	3:48pm
CAL	Pass	3:48pm

Preventive Maintenance
Status: Pass

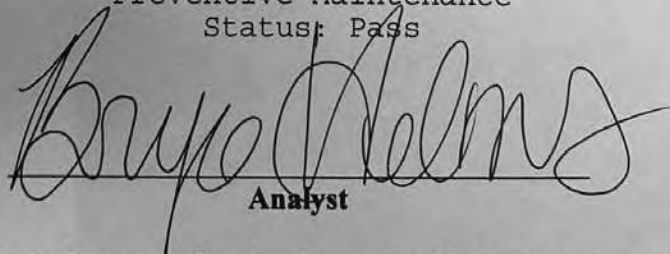

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location Huntersville PD
Instrument Serial No. 008797 Huntersville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: 008747

Test Date: 02/01/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	1:47pm
AIR BLK	.00	1:48pm
ACCY CHK	.08	1:48pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:53pm
AIR BLK	.00	1:53pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: 008747 Test Record Number: 2908
Test Date: 02/01/2022 Test Time: 1:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:54pm
FLO	Pass	1:54pm
FC	Pass	1:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:55pm

CRC Tests

Test	Status	Time
COMP	Pass	1:55pm
CAL	Pass	1:55pm

Preventive Maintenance
Status: Pass

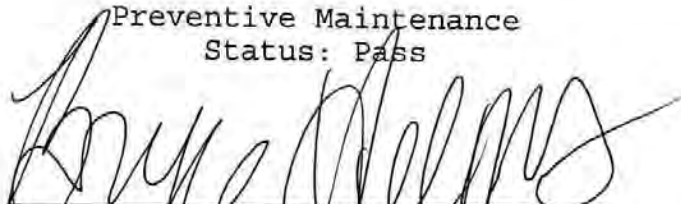

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT MOBILE UNIT 2
Instrument Serial No. 008970 Matthews

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

673
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG BAT MOBILE UNIT 2 590

Serial Number: 008970
Test Date: 02/18/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barrier II, Dennis J

Permit Number: 0014-7953

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	8:32pm
AIR BLK	.00	8:33pm
ACCY CHK	.08	8:33pm
AIR BLK	.00	8:34pm
SUB TEST	.00	8:35pm
AIR BLK	.00	8:36pm
SUB TEST	.00	8:37pm
AIR BLK	.00	8:38pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG BAT MOBILE UNIT 2 590

Serial Number: 008970 Test Record Number: 863
Test Date: 02/18/2022 Test Time: 8:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:39pm
FLO	Pass	8:39pm
FC	Pass	8:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:40pm
SRC	Pass	8:40pm
DET	Pass	8:40pm
BAR	Pass	8:40pm
BT	Pass	8:40pm

Blank Tests

Test	Status	Time
AIR	Pass	8:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:40pm

CRC Tests

Test	Status	Time
COMP	Pass	8:40pm
CAL	Pass	8:40pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT MOBILE UNIT 2
Instrument Serial No. 008973 Matthews

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

673
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG BAT MOBILE UNIT 2 590

Serial Number: 008973
Test Date: 02/18/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barrier II, Dennis J

Permit Number: 0014-7953

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA


Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	8:34pm
AIR BLK	.00	8:35pm
ACCY CHK	.08	8:35pm
AIR BLK	.00	8:36pm
SUB TEST	.00	8:37pm
AIR BLK	.00	8:37pm
SUB TEST	.00	8:39pm
AIR BLK	.00	8:40pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG BAT MOBILE UNIT 2 590

Serial Number: 008973 Test Record Number: 944
Test Date: 02/18/2022 Test Time: 8:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:41pm
FLO	Pass	8:41pm
FC	Pass	8:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:41pm
SRC	Pass	8:41pm
DET	Pass	8:41pm
BAR	Pass	8:41pm
BT	Pass	8:41pm

Blank Tests

Test	Status	Time
AIR	Pass	8:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:42pm

CRC Tests

Test	Status	Time
COMP	Pass	8:42pm
CAL	Pass	8:42pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NASH Instrument Location NAT MOBILE UNIT 6

Instrument Serial No. 008580 SHARPSAVAL

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008580

Test Date: 02/23/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS\


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	9:27pm
AIR BLK	.00	9:28pm
ACCY CHK	.07	9:29pm
AIR BLK	.00	9:30pm
SUB TEST	.00	9:30pm
AIR BLK	.00	9:31pm
SUB TEST	.00	9:32pm
AIR BLK	.00	9:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008580 Test Record Number: 2689
Test Date: 02/23/2022 Test Time: 9:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:36pm
FLO	Pass	9:36pm
FC	Pass	9:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:36pm
SRC	Pass	9:36pm
DET	Pass	9:36pm
BAR	Pass	9:36pm
BT	Pass	9:36pm

Blank Tests

Test	Status	Time
AIR	Pass	9:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:37pm

CRC Tests

Test	Status	Time
COMP	Pass	9:37pm
CAL	Pass	9:37pm

Preventive Maintenance
Status: Pass

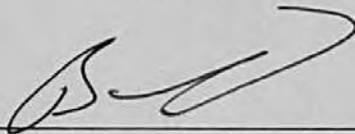

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NEW HANOVER Instrument Location WILMINGTON
Instrument Serial No. 008628 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Berry
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY WILMINGTON PD 640

Serial Number: 008628

Test Date: 02/22/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG131901


Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	3:12pm
AIR BLK	.00	3:13pm
ACCY CHK	.08	3:14pm
AIR BLK	.00	3:15pm
SUB TEST	.00	3:16pm
AIR BLK	.00	3:17pm
SUB TEST	.00	3:18pm
AIR BLK	.00	3:19pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY WILMINGTON PD 640

Serial Number: 008628 Test Record Number: 5837
Test Date: 02/22/2022 Test Time: 3:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:22pm
FLO	Pass	3:22pm
FC	Pass	3:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:22pm
SRC	Pass	3:22pm
DET	Pass	3:22pm
BAR	Pass	3:22pm
BT	Pass	3:22pm

Blank Tests

Test	Status	Time
AIR	Pass	3:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:23pm

CRC Tests

Test	Status	Time
COMP	Pass	3:23pm
CAL	Pass	3:23pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Northampton Instrument Location Northampton Co. S.O.
Instrument Serial No. 008607 105 West Johnson St
Jackson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. B. Bryant
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT
650

Serial Number: 008607
Test Date: 02/24/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	12:54pm
AIR BLK	.00	12:54pm
ACCY CHK	.07	12:55pm
AIR BLK	.00	12:56pm
SUB TEST	.00	12:57pm
AIR BLK	.00	12:58pm
SUB TEST	.00	1:00pm
AIR BLK	.00	1:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

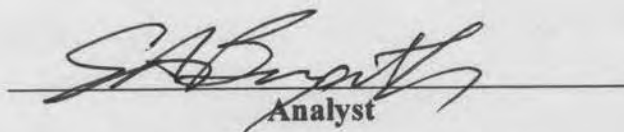

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650

Serial Number: 008607 Test Record Number: 1145
Test Date: 02/24/2022 Test Time: 1:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:02pm
FLO	Pass	1:02pm
FC	Pass	1:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:02pm
SRC	Pass	1:02pm
DET	Pass	1:02pm
BAR	Pass	1:02pm
BT	Pass	1:02pm

Blank Tests

Test	Status	Time
AIR	Pass	1:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:03pm

CRC Tests

Test	Status	Time
COMP	Pass	1:03pm
CAL	Pass	1:03pm

Preventive Maintenance
Status: Pass

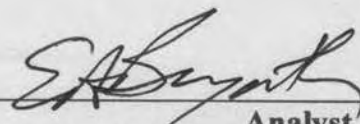

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Northampton Instrument Location Northampton Co. S.O.
Instrument Serial No. DD8688 105 West Jefferson St
Jackson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



EAB
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT
650

Serial Number: 008688
Test Date: 02/24/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	12:59pm
AIR BLK	.00	1:00pm
ACCY CHK	.07	1:01pm
AIR BLK	.00	1:02pm
SUB TEST	.00	1:02pm
AIR BLK	.00	1:03pm
SUB TEST	.00	1:05pm
AIR BLK	.00	1:06pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650

Serial Number: 008688 Test Record Number: 978
Test Date: 02/24/2022 Test Time: 1:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:07pm
FLO	Pass	1:07pm
FC	Pass	1:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:07pm
SRC	Pass	1:07pm
DET	Pass	1:07pm
BAR	Pass	1:07pm
BT	Pass	1:07pm

Blank Tests

Test	Status	Time
AIR	Pass	1:08pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:08pm

CRC Tests

Test	Status	Time
COMP	Pass	1:08pm
CAL	Pass	1:08pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ms Low County Instrument Location BAT mobile
Instrument Serial No. 008380 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

678
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008580
Test Date: 02/13/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Douglas, Glen E

Permit Number: 6141-3926

Effective:

02/01/2022-02/01/2024

Officer's Name: Douglas, Glen E

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	11:22pm
AIR BLK	.00	11:23pm
ACCY CHK	.07	11:23pm
AIR BLK	.00	11:24pm
SUB TEST	.00	11:25pm
AIR BLK	.00	11:25pm
SUB TEST	.00	11:27pm
AIR BLK	.00	11:28pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008580 Test Record Number: 2685
Test Date: 02/13/2022 Test Time: 11:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:29pm
FLO	Pass	11:29pm
FC	Pass	11:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:29pm
SRC	Pass	11:29pm
DET	Pass	11:29pm
BAR	Pass	11:29pm
BT	Pass	11:29pm

Blank Tests

Test	Status	Time
AIR	Pass	11:30pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:30pm

CRC Tests

Test	Status	Time
COMP	Pass	11:30pm
CAL	Pass	11:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MSLOW County Instrument Location BAT mobile
Instrument Serial No. 008584 JACKSONVILLE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

678
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

.Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008584
Test Date: 02/13/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Douglas, Glen E

Permit Number: 6141-3926

Effective:

02/01/2022-02/01/2024

Officer's Name: Douglas, Glen E

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	10:52pm
AIR BLK	.00	10:52pm
ACCY CHK	.07	10:53pm
AIR BLK	.00	10:54pm
SUB TEST	.00	10:54pm
AIR BLK	.00	10:55pm
SUB TEST	.00	10:56pm
AIR BLK	.00	10:57pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008584 Test Record Number: 2419
Test Date: 02/13/2022 Test Time: 10:58pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:58pm
FLO	Pass	10:58pm
FC	Pass	10:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:58pm
SRC	Pass	10:58pm
DET	Pass	10:58pm
BAR	Pass	10:58pm
BT	Pass	10:58pm

Blank Tests

Test	Status	Time
AIR	Pass	10:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:59pm

CRC Tests

Test	Status	Time
COMP	Pass	10:59pm
CAL	Pass	10:59pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location BAT Mobile Unit 12

Instrument Serial No. 009600 Sneeds Ferry

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. G. [Signature]
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE 12 660

Serial Number: 008600 Test Record Number: 2178
Test Date: 02/03/2022 Test Time: 11:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:12pm
FLO	Pass	11:12pm
FC	Pass	11:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:13pm
SRC	Pass	11:13pm
DET	Pass	11:13pm
BAR	Pass	11:13pm
BT	Pass	11:13pm

Blank Tests

Test	Status	Time
AIR	Pass	11:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:13pm

CRC Tests

Test	Status	Time
COMP	Pass	11:13pm
CAL	Pass	11:13pm

Preventive Maintenance
Status: Pass

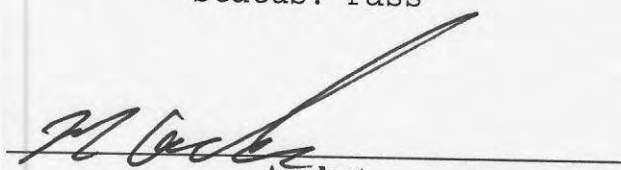

Analyst

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE 12 660

Serial Number: 008600
Test Date: 02/03/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	11:04pm
AIR BLK	.00	11:05pm
ACCY CHK	.08	11:06pm
AIR BLK	.00	11:07pm
SUB TEST	.00	11:08pm
AIR BLK	.00	11:09pm
SUB TEST	.00	11:10pm
AIR BLK	.00	11:11pm

Reported AC: 00 g/210L

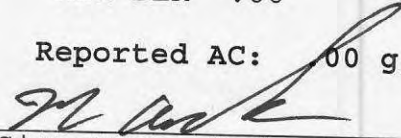

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow County Instrument Location BAT Mobile
Instrument Serial No. 008637 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

678
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008637

Test Date: 02/13/2022

Citation Number: M0000000-0

Subject's Name: PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Douglas, Glen E

Permit Number: 6141-3926

Effective:

02/01/2022-02/01/2024

Officer's Name: Douglas, Glen E

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	9:16pm
AIR BLK	.00	9:17pm
ACCY CHK	.07	9:18pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:19pm
AIR BLK	.00	9:21pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:25pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008637 Test Record Number: 3189
Test Date: 02/13/2022 Test Time: 9:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:31pm
FLO	Pass	9:31pm
FC	Pass	9:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:31pm
SRC	Pass	9:31pm
DET	Pass	9:31pm
BAR	Pass	9:31pm
BT	Pass	9:31pm

Blank Tests

Test	Status	Time
AIR	Pass	9:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:31pm

CRC Tests

Test	Status	Time
COMP	Pass	9:32pm
CAL	Pass	9:32pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow County Instrument Location BAT mobile
Instrument Serial No. 008686 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

678
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008686

Test Date: 02/13/2022

Citation Number: M0000000-0

Subject's Name: PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Douglas, Glen E

Permit Number: 6141-3926

Effective:

02/01/2022-02/01/2024

Officer's Name: Douglas, Glen E

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	9:14pm
AIR BLK	.00	9:15pm
ACCY CHK	.08	9:16pm
AIR BLK	.00	9:17pm
SUB TEST	.00	9:18pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:21pm
AIR BLK	.00	9:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008686 Test Record Number: 6836
Test Date: 02/13/2022 Test Time: 9:28pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:28pm
FLO	Pass	9:28pm
FC	Pass	9:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:29pm
SRC	Pass	9:29pm
DET	Pass	9:29pm
BAR	Pass	9:29pm
BT	Pass	9:29pm

Blank Tests

Test	Status	Time
AIR	Pass	9:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:29pm

CRC Tests

Test	Status	Time
COMP	Pass	9:29pm
CAL	Pass	9:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location BAT mobile
Instrument Serial No. 008776 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

678
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008776

Test Date: 02/13/2022

Citation Number: M0000000-0

Subject's Name: PREVENTIVE, MAINTENCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Douglas, Glen E

Permit Number: 6141-3926

Effective:

02/01/2022-02/01/2024

Officer's Name: Douglas, Glen E

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	9:12pm
AIR BLK	.00	9:13pm
ACCY CHK	.07	9:14pm
AIR BLK	.00	9:15pm
SUB TEST	.00	9:15pm
AIR BLK	.00	9:16pm
SUB TEST	.00	9:18pm
AIR BLK	.00	9:19pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008776 Test Record Number: 3739
Test Date: 02/13/2022 Test Time: 9:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:20pm
FLO	Pass	9:20pm
FC	Pass	9:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:20pm
SRC	Pass	9:20pm
DET	Pass	9:20pm
BAR	Pass	9:20pm
BT	Pass	9:20pm

Blank Tests

Test	Status	Time
AIR	Pass	9:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:21pm

CRC Tests

Test	Status	Time
COMP	Pass	9:21pm
CAL	Pass	9:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MSLOW County Instrument Location BAT mobile
Instrument Serial No. 008779 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

678
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008779
Test Date: 02/13/2022

Citation Number: M0000000-0
Subject's Name: PREVENTIVE, MAINTENCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Douglas, Glen E
Permit Number: 6141-3926
Effective:
02/01/2022-02/01/2024

Officer's Name: Douglas, Glen E
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG035001
Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	10:14pm
AIR BLK	.00	10:15pm
ACCY CHK	.07	10:15pm
AIR BLK	.00	10:16pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008779 Test Record Number: 3758
Test Date: 02/13/2022 Test Time: 10:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:11pm
FLO	Pass	10:11pm
FC	Pass	10:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:11pm
SRC	Pass	10:11pm
DET	Pass	10:11pm
BAR	Pass	10:11pm
BT	Pass	10:11pm

Blank Tests

Test	Status	Time
AIR	Pass	10:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:12pm

CRC Tests

Test	Status	Time
COMP	Pass	10:12pm
CAL	Pass	10:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Onslow Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008788 Sneads Ferry

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008788
Test Date: 02/03/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	10:59pm
AIR BLK	.00	11:00pm
ACCY CHK	.08	11:00pm
AIR BLK	.00	11:01pm
SUB TEST	.00	11:02pm
AIR BLK	.00	11:03pm
SUB TEST	.00	11:04pm
AIR BLK	.00	11:05pm

Reported AC: .00 g/210L

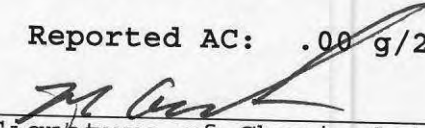

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008788 Test Record Number: 1725
Test Date: 02/03/2022 Test Time: 11:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07pm
FLO	Pass	11:07pm
FC	Pass	11:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:07pm
SRC	Pass	11:07pm
DET	Pass	11:07pm
BAR	Pass	11:07pm
BT	Pass	11:07pm

Blank Tests

Test	Status	Time
AIR	Pass	11:08pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:08pm

CRC Tests

Test	Status	Time
COMP	Pass	11:08pm
CAL	Pass	11:08pm

Preventive Maintenance
Status: Pass

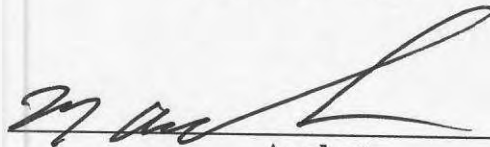

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLow Instrument Location MCAS NEW RIVER
Instrument Serial No. 008919 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bauer
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ON SLOW COUNTY MCAS NEW RIVER 660

Serial Number: 008919
Test Date: 02/28/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG131901
Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	5:12pm
AIR BLK	.00	5:12pm
ACCY CHK	.07	5:13pm
AIR BLK	.00	5:14pm
SUB TEST	.00	5:15pm
AIR BLK	.00	5:16pm
SUB TEST	.00	5:17pm
AIR BLK	.00	5:18pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919 Test Record Number: 793
Test Date: 02/28/2022 Test Time: 5:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:19pm
FLO	Pass	5:19pm
FC	Pass	5:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:19pm
SRC	Pass	5:19pm
DET	Pass	5:19pm
BAR	Pass	5:19pm
BT	Pass	5:19pm

Blank Tests

Test	Status	Time
AIR	Pass	5:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:20pm

CRC Tests

Test	Status	Time
COMP	Pass	5:20pm
CAL	Pass	5:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSLOW Instrument Location CAMP LEJEUNE
Instrument Serial No. 008920 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920
Test Date: 02/28/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG131901
Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	2:47pm
AIR BLK	.00	2:48pm
ACCY CHK	.08	2:49pm
AIR BLK	.00	2:50pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm
SUB TEST	.00	2:53pm
AIR BLK	.00	2:54pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920 Test Record Number: 1971
Test Date: 02/28/2022 Test Time: 2:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:54pm
FLO	Pass	2:54pm
FC	Pass	2:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:54pm
SRC	Pass	2:54pm
DET	Pass	2:54pm
BAR	Pass	2:54pm
BT	Pass	2:54pm

Blank Tests

Test	Status	Time
AIR	Pass	2:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:55pm

CRC Tests

Test	Status	Time
COMP	Pass	2:55pm
CAL	Pass	2:55pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSLOW Instrument Location JACKSONVILLE
Instrument Serial No. 008930 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY JACKSONVILLE PD 660

Serial Number: 008930
Test Date: 02/28/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:37pm
AIR BLK	.00	1:38pm
ACCY CHK	.08	1:38pm
AIR BLK	.00	1:39pm
SUB TEST	.00	1:40pm
AIR BLK	.00	1:41pm
SUB TEST	.00	1:43pm
AIR BLK	.00	1:43pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY JACKSONVILLE PD 660

Serial Number: 008930 Test Record Number: 2145
Test Date: 02/28/2022 Test Time: 1:44pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:44pm
FLO	Pass	1:44pm
FC	Pass	1:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:44pm
SRC	Pass	1:44pm
DET	Pass	1:44pm
BAR	Pass	1:44pm
BT	Pass	1:44pm

Blank Tests

Test	Status	Time
AIR	Pass	1:45pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:45pm

CRC Tests

Test	Status	Time
COMP	Pass	1:45pm
CAL	Pass	1:45pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSLOW Instrument Location ONSLOW COUNTY

Instrument Serial No. 008931 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Banco
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931
Test Date: 02/28/2022

Citation Number: M0000000-0

Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	12:21pm
AIR BLK	.00	12:21pm
ACCY CHK	.08	12:22pm
AIR BLK	.00	12:23pm
SUB TEST	.00	12:24pm
AIR BLK	.00	12:25pm
SUB TEST	.00	12:26pm
AIR BLK	.00	12:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931 Test Record Number: 3820
Test Date: 02/28/2022 Test Time: 12:27pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:28pm
FLO	Pass	12:28pm
FC	Pass	12:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:28pm
SRC	Pass	12:28pm
DET	Pass	12:28pm
BAR	Pass	12:28pm
BT	Pass	12:28pm

Blank Tests

Test	Status	Time
AIR	Pass	12:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:29pm

CRC Tests

Test	Status	Time
COMP	Pass	12:29pm
CAL	Pass	12:29pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLow Instrument Location ONSLow COUNTY
Instrument Serial No. 008932 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bando
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008932
Test Date: 02/28/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	12:30pm
AIR BLK	.00	12:30pm
ACCY CHK	.08	12:31pm
AIR BLK	.00	12:32pm
SUB TEST	.00	12:34pm
AIR BLK	.00	12:34pm
SUB TEST	.00	12:36pm
AIR BLK	.00	12:37pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLow COUNTY DETENTION CENTER 660

Serial Number: 008932 Test Record Number: 6639
Test Date: 02/28/2022 Test Time: 12:37pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:37pm
FLO	Pass	12:37pm
FC	Pass	12:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:38pm
SRC	Pass	12:38pm
DET	Pass	12:38pm
BAR	Pass	12:38pm
BT	Pass	12:38pm

Blank Tests

Test	Status	Time
AIR	Pass	12:38pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:38pm

CRC Tests

Test	Status	Time
COMP	Pass	12:39pm
CAL	Pass	12:39pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ORANGE Instrument Location Chapel Hill PD
Instrument Serial No. 008839 828 Martin Luther King Blvd
Chapel Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

471
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: 008839

Test Date: 02/03/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107502

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	11:23am
AIR BLK	.00	11:23am
ACCY CHK	.08	11:24am
AIR BLK	.00	11:25am
SUB TEST	.00	11:26am
AIR BLK	.00	11:27am
SUB TEST	.00	11:28am
AIR BLK	.00	11:29am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: 008839 Test Record Number: 2473
Test Date: 02/03/2022 Test Time: 11:32am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:32am
FLO	Pass	11:32am
FC	Pass	11:32am

Temperature Tests

Test	Status	Time
FC1	Pass	11:33am
SRC	Pass	11:33am
DET	Pass	11:33am
BAR	Pass	11:33am
BT	Pass	11:33am

Blank Tests

Test	Status	Time
AIR	Pass	11:33am

Printer Tests

Test	Status	Time
PRNT	Pass	11:33am

CRC Tests

Test	Status	Time
COMP	Pass	11:33am
CAL	Pass	11:33am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ORANGE Instrument Location Chapel Hill PD

Instrument Serial No. 058856 828 Martin Lane King Road

Chapel Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: 008856

Test Date: 02/22/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	7:09am
AIR BLK	.00	7:10am
ACCY CHK	.07	7:10am
AIR BLK	.00	7:11am
SUB TEST	.00	7:11am
AIR BLK	.00	7:12am
SUB TEST	.00	7:14am
AIR BLK	.00	7:15am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: 008856 Test Record Number: 2807
Test Date: 02/22/2022 Test Time: 7:15am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:15am
FLO	Pass	7:15am
FC	Pass	7:15am

Temperature Tests

Test	Status	Time
FC1	Pass	7:15am
SRC	Pass	7:15am
DET	Pass	7:15am
BAR	Pass	7:15am
BT	Pass	7:15am

Blank Tests

Test	Status	Time
AIR	Pass	7:16am

Printer Tests

Test	Status	Time
PRNT	Pass	7:16am

CRC Tests

Test	Status	Time
COMP	Pass	7:16am
CAL	Pass	7:16am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Person Instrument Location Person Co LEC
Instrument Serial No. 003693 120 Court St Person NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008693
Test Date: 02/07/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

09/01/2020-09/01/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401


Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	6:59pm
AIR BLK	.00	7:00pm
ACCY CHK	.07	7:00pm
AIR BLK	.00	7:01pm
SUB TEST	.00	7:02pm
AIR BLK	.00	7:03pm
SUB TEST	.00	7:05pm
AIR BLK	.00	7:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008693 Test Record Number: 1872
Test Date: 02/07/2022 Test Time: 7:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:08pm
FLO	Pass	7:08pm
FC	Pass	7:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:08pm
SRC	Pass	7:08pm
DET	Pass	7:08pm
BAR	Pass	7:08pm
BT	Pass	7:08pm

Blank Tests

Test	Status	Time
AIR	Pass	7:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:09pm

CRC Tests

Test	Status	Time
COMP	Pass	7:09pm
CAL	Pass	7:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Person Instrument Location Person Co LEC

Instrument Serial No. 009480 120 Cant St Person, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Emmanuel A. [Signature] 682
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008880

Test Date: 02/07/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

09/01/2020-09/01/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401


Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	7:00pm
AIR BLK	.00	7:00pm
ACCY CHK	.07	7:01pm
AIR BLK	.00	7:02pm
SUB TEST	.00	7:03pm
AIR BLK	.00	7:03pm
SUB TEST	.00	7:05pm
AIR BLK	.00	7:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY PERSON CO. LEC 720

Serial Number: 008880 Test Record Number: 1845
Test Date: 02/07/2022 Test Time: 7:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:08pm
FLO	Pass	7:08pm
FC	Pass	7:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:08pm
SRC	Pass	7:08pm
DET	Pass	7:08pm
BAR	Pass	7:08pm
BT	Pass	7:08pm

Blank Tests

Test	Status	Time
AIR	Pass	7:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:09pm

CRC Tests

Test	Status	Time
COMP	Pass	7:09pm
CAL	Pass	7:09pm

Preventive Maintenance
Status: *Pass*

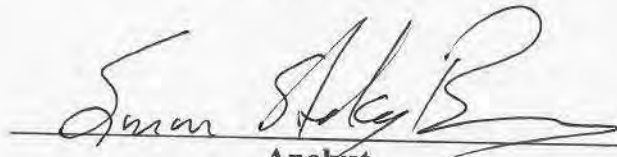
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County P.H. Instrument Location Ayden P.D.

Instrument Serial No. 00960606 4144 West Ave, Ayden, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY AYDEN PD 730

Serial Number: 008666
Test Date: 02/08/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023


Test	g/210L	Time
DIAG	Pass	2:46pm
AIR BLK	.00	2:47pm
ACCY CHK	.07	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:49pm
AIR BLK	.00	2:50pm
SUB TEST	.00	2:52pm
AIR BLK	.00	2:53pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY AYDEN PD 730

Serial Number: 008666 Test Record Number: 1399
Test Date: 02/08/2022 Test Time: 2:55pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:55pm
FLO	Pass	2:55pm
FC	Pass	2:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:55pm
SRC	Pass	2:55pm
DET	Pass	2:55pm
BAR	Pass	2:55pm
BT	Pass	2:55pm

Blank Tests

Test	Status	Time
AIR	Pass	2:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:56pm

CRC Tests

Test	Status	Time
COMP	Pass	2:56pm
CAL	Pass	2:56pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Randolph Instrument Location Randleman Police
Instrument Serial No. 008737 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: 008737
Test Date: 02/21/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Garner, Joel K*
Permit Number: 0036-5156
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG118803
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	1:12pm
AIR BLK	.00	1:13pm
ACCY CHK	.08	1:13pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:15pm
AIR BLK	.00	1:16pm
SUB TEST	.00	1:17pm
AIR BLK	.00	1:18pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: 008737 Test Record Number: 1341
Test Date: 02/21/2022 Test Time: 1:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:19pm
FLO	Pass	1:19pm
FC	Pass	1:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:20pm
SRC	Pass	1:20pm
DET	Pass	1:20pm
BAR	Pass	1:20pm
BT	Pass	1:20pm

Blank Tests

Test	Status	Time
AIR	Pass	1:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:20pm

CRC Tests

Test	Status	Time
COMP	Pass	1:20pm
CAL	Pass	1:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Randolph Instrument Location Liberty Police
Instrument Serial No. 008830 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830
Test Date: 02/21/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023


Test	g/210L	Time
DIAG	Pass	2:12pm
AIR BLK	.00	2:13pm
ACCY CHK	.08	2:13pm
AIR BLK	.00	2:15pm
SUB TEST	.00	2:15pm
AIR BLK	.00	2:16pm
SUB TEST	.00	2:18pm
AIR BLK	.00	2:19pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830 Test Record Number: 748
Test Date: 02/21/2022 Test Time: 2:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:20pm
FLO	Pass	2:20pm
FC	Pass	2:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:20pm
SRC	Pass	2:20pm
DET	Pass	2:20pm
BAR	Pass	2:20pm
BT	Pass	2:20pm

Blank Tests

Test	Status	Time
AIR	Pass	2:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:21pm

CRC Tests

Test	Status	Time
COMP	Pass	2:21pm
CAL	Pass	2:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Randolph Instrument Location Randolph County

Instrument Serial No. 008860 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: 008860
Test Date: 02/21/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	11:46am
AIR BLK	.00	11:47am
ACCY CHK	.08	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:49am
AIR BLK	.00	11:50am
SUB TEST	.00	11:51am
AIR BLK	.00	11:52am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: 008860 Test Record Number: 3085
Test Date: 02/21/2022 Test Time: 11:53am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:54am
FLO	Pass	11:54am
FC	Pass	11:54am

Temperature Tests

Test	Status	Time
FC1	Pass	11:54am
SRC	Pass	11:54am
DET	Pass	11:54am
BAR	Pass	11:54am
BT	Pass	11:54am

Blank Tests

Test	Status	Time
AIR	Pass	11:54am


Printer Tests

Test	Status	Time
PRNT	Pass	11:54am

CRC Tests

Test	Status	Time
COMP	Pass	11:55am
CAL	Pass	11:55am

Preventive Maintenance
Status: Pass

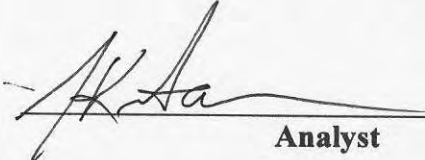

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Randolph Instrument Location Randolph County
Instrument Serial No. 008899 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: 008899

Test Date: 02/21/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118803

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	11:47am
AIR BLK	.00	11:48am
ACCY CHK	.08	11:49am
AIR BLK	.00	11:50am
SUB TEST	.00	11:50am
AIR BLK	.00	11:51am
SUB TEST	.00	11:52am
AIR BLK	.00	11:53am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: 008899 Test Record Number: 3809
Test Date: 02/21/2022 Test Time: 11:54am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:54am
FLO	Pass	11:54am
FC	Pass	11:54am

Temperature Tests

Test	Status	Time
FC1	Pass	11:54am
SRC	Pass	11:54am
DET	Pass	11:54am
BAR	Pass	11:54am
BT	Pass	11:54am

Blank Tests

Test	Status	Time
AIR	Pass	11:55am

Printer Tests

Test	Status	Time
PRNT	Pass	11:55am

CRC Tests

Test	Status	Time
COMP	Pass	11:55am
CAL	Pass	11:55am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County RANDOLPH Instrument Location ARCHDALE POLICE

Instrument Serial No. 008791 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY ARCHDALE PD 750

Serial Number: 008791
Test Date: 02/14/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118803

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	2:17pm
AIR BLK	.00	2:18pm
ACCY CHK	.08	2:19pm
AIR BLK	.00	2:20pm
SUB TEST	.00	2:20pm
AIR BLK	.00	2:21pm
SUB TEST	.00	2:23pm
AIR BLK	.00	2:24pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY ARCHDALE PD 750

Serial Number: 008791 Test Record Number: 1490
Test Date: 02/14/2022 Test Time: 2:25pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:25pm
FLO	Pass	2:25pm
FC	Pass	2:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:25pm
SRC	Pass	2:25pm
DET	Pass	2:25pm
BAR	Pass	2:25pm
BT	Pass	2:25pm

Blank Tests

Test	Status	Time
AIR	Pass	2:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:26pm

CRC Tests

Test	Status	Time
COMP	Pass	2:26pm
CAL	Pass	2:26pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location Pembroke Police

Instrument Serial No. 008863 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY PEMBROKE POLICE DEPT
770

Serial Number: 008863
Test Date: 02/22/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG132001
Exp Date: 11/16/2023


Test	g/210L	Time
DIAG	Pass	11:17am
AIR BLK	.00	11:17am
ACCY CHK	.07	11:18am
AIR BLK	.00	11:19am
SUB TEST	.00	11:20am
AIR BLK	.00	11:21am
SUB TEST	.00	11:23am
AIR BLK	.00	11:23am

Reported AC: .00 g/210L

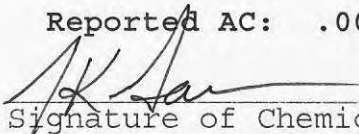

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY PEMBROKE POLICE DEPT 770

Serial Number: 008863 Test Record Number: 844
Test Date: 02/22/2022 Test Time: 11:24am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:25am
FLO	Pass	11:25am
FC	Pass	11:25am

Temperature Tests

Test	Status	Time
FC1	Pass	11:25am
SRC	Pass	11:25am
DET	Pass	11:25am
BAR	Pass	11:25am
BT	Pass	11:25am

Blank Tests

Test	Status	Time
AIR	Pass	11:25am


Printer Tests

Test	Status	Time
PRNT	Pass	11:26am

CRC Tests

Test	Status	Time
COMP	Pass	11:26am
CAL	Pass	11:26am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Robeson Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008575 Robeson Co. S.O.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

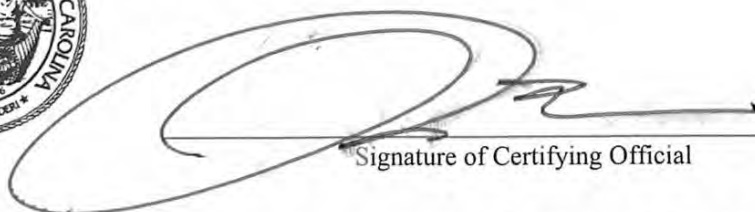


Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008575
Test Date: 02/18/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

06/08/2020-06/08/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	9:35pm
AIR BLK	.00	9:36pm
ACCY CHK	.08	9:37pm
AIR BLK	.00	9:38pm
SUB TEST	.00	9:38pm
AIR BLK	.00	9:39pm
SUB TEST	.00	9:41pm
AIR BLK	.00	9:42pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008575 Test Record Number: 1298
Test Date: 02/18/2022 Test Time: 9:44pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:45pm
FLO	Pass	9:45pm
FC	Pass	9:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:45pm
SRC	Pass	9:45pm
DET	Pass	9:45pm
BAR	Pass	9:45pm
BT	Pass	9:45pm

Blank Tests

Test	Status	Time
AIR	Pass	9:46pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:46pm

CRC Tests

Test	Status	Time
COMP	Pass	9:46pm
CAL	Pass	9:46pm

Preventive Maintenance
Status: Pass

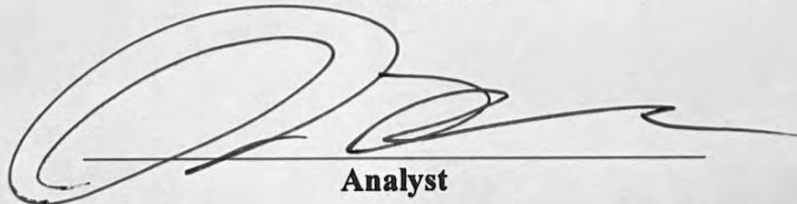

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008707 Robeson Co.S.O.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008707
Test Date: 02/18/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

06/08/2020-06/08/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501


Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	9:40pm
AIR BLK	.00	9:41pm
ACCY CHK	.08	9:41pm
AIR BLK	.00	9:42pm
SUB TEST	.00	9:43pm
AIR BLK	.00	9:44pm
SUB TEST	.00	9:45pm
AIR BLK	.00	9:46pm

Reported AC: .00 g/210L

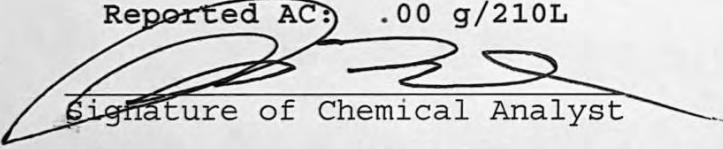
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008707 Test Record Number: 2719
Test Date: 02/18/2022 Test Time: 9:50pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:50pm
FLO	Pass	9:50pm
FC	Pass	9:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:50pm
SRC	Pass	9:50pm
DET	Pass	9:50pm
BAR	Pass	9:50pm
BT	Pass	9:50pm

Blank Tests

Test	Status	Time
AIR	Pass	9:51pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:51pm

CRC Tests

Test	Status	Time
COMP	Pass	9:51pm
CAL	Pass	9:51pm

Preventive Maintenance
Status: Pass

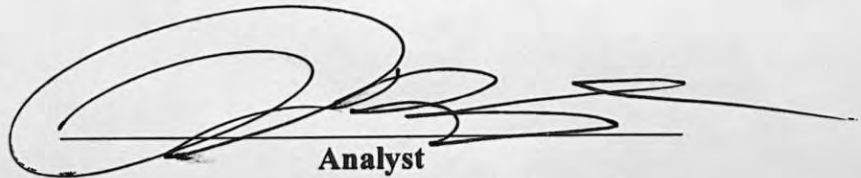

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROCKINGHAM Instrument Location EDEW POLICE

Instrument Serial No. 008636 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636
Test Date: 02/08/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118803

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	9:13am
AIR BLK	.00	9:14am
ACCY CHK	.08	9:15am
AIR BLK	.00	9:16am
SUB TEST	.00	9:17am
AIR BLK	.00	9:18am
SUB TEST	.00	9:19am
AIR BLK	.00	9:20am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636 Test Record Number: 2289
Test Date: 02/08/2022 Test Time: 9:24am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:24am
FLO	Pass	9:24am
FC	Pass	9:24am

Temperature Tests

Test	Status	Time
FC1	Pass	9:24am
SRC	Pass	9:24am
DET	Pass	9:24am
BAR	Pass	9:24am
BT	Pass	9:24am

Blank Tests

Test	Status	Time
AIR	Pass	9:25am

Printer Tests

Test	Status	Time
PRNT	Pass	9:25am

CRC Tests

Test	Status	Time
COMP	Pass	9:25am
CAL	Pass	9:25am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROCKINGHAM Instrument Location REIDSVILLE POLICE

Instrument Serial No. 008784 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: 008784
Test Date: 02/08/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	10:13am
AIR BLK	.00	10:14am
ACCY CHK	.08	10:14am
AIR BLK	.00	10:16am
SUB TEST	.00	10:16am
AIR BLK	.00	10:17am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: 008784 Test Record Number: 1315
Test Date: 02/08/2022 Test Time: 10:20am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:21am
FLO	Pass	10:21am
FC	Pass	10:21am

Temperature Tests

Test	Status	Time
FC1	Pass	10:21am
SRC	Pass	10:21am
DET	Pass	10:21am
BAR	Pass	10:21am
BT	Pass	10:21am

Blank Tests

Test	Status	Time
AIR	Pass	10:22am


Printer Tests

Test	Status	Time
PRNT	Pass	10:22am

CRC Tests

Test	Status	Time
COMP	Pass	10:22am
CAL	Pass	10:22am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROWAN Instrument Location SALISBURY POLICE

Instrument Serial No. 008835 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835
Test Date: 02/15/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	8:57am
AIR BLK	.00	8:58am
ACCY CHK	.08	8:59am
AIR BLK	.00	9:00am
SUB TEST	.00	9:01am
AIR BLK	.00	9:02am
SUB TEST	.00	9:03am
AIR BLK	.00	9:04am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835 Test Record Number: 2824
Test Date: 02/15/2022 Test Time: 9:05am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:06am
FLO	Pass	9:06am
FC	Pass	9:06am

Temperature Tests

Test	Status	Time
FC1	Pass	9:06am
SRC	Pass	9:06am
DET	Pass	9:06am
BAR	Pass	9:06am
BT	Pass	9:06am

Blank Tests

Test	Status	Time
AIR	Pass	9:07am

Printer Tests

Test	Status	Time
PRNT	Pass	9:07am

CRC Tests

Test	Status	Time
COMP	Pass	9:07am
CAL	Pass	9:07am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROWAN Instrument Location SALISBURY POLICE

Instrument Serial No. 008868 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868
Test Date: 02/15/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	8:54am
AIR BLK	.00	8:55am
ACCY CHK	.08	8:56am
AIR BLK	.00	8:57am
SUB TEST	.00	8:58am
AIR BLK	.00	8:59am
SUB TEST	.00	9:00am
AIR BLK	.00	9:01am

Reported AC: .00 g/210L

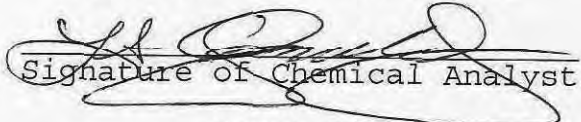
Signature of Chemical Analyst
Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868 Test Record Number: 3365
Test Date: 02/15/2022 Test Time: 9:02am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:03am
FLO	Pass	9:03am
FC	Pass	9:03am

Temperature Tests

Test	Status	Time
FC1	Pass	9:03am
SRC	Pass	9:03am
DET	Pass	9:03am
BAR	Pass	9:03am
BT	Pass	9:03am

Blank Tests

Test	Status	Time
AIR	Pass	9:04am

Printer Tests

Test	Status	Time
PRNT	Pass	9:04am

CRC Tests

Test	Status	Time
COMP	Pass	9:04am
CAL	Pass	9:04am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Sampson Instrument Location BAT mobile Unit #5
Instrument Serial No. 008647 Sampson County Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

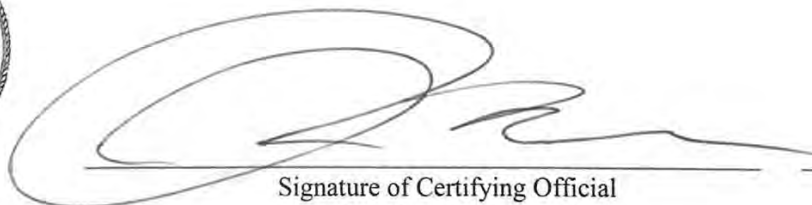


Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008647

Test Date: 02/03/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

06/08/2020-06/08/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG132002


Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	9:21pm
AIR BLK	.00	9:22pm
ACCY CHK	.08	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:27pm
AIR BLK	.00	9:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

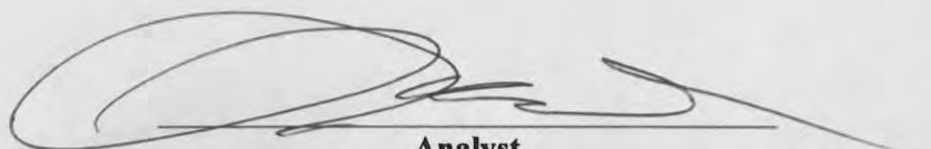
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 5 810
Serial Number: 008647 Test Record Number: 2680
Test Date: 02/03/2022 Test Time: 9:29pm EST
System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:29pm
FLO	Pass	9:29pm
FC	Pass	9:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:29pm
SRC	Pass	9:29pm
DET	Pass	9:29pm
BAR	Pass	9:29pm
BT	Pass	9:29pm

Blank Tests

Test	Status	Time
AIR	Pass	9:30pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:30pm

CRC Tests

Test	Status	Time
COMP	Pass	9:30pm
CAL	Pass	9:30pm

Preventive Maintenance
Status: *Pass*

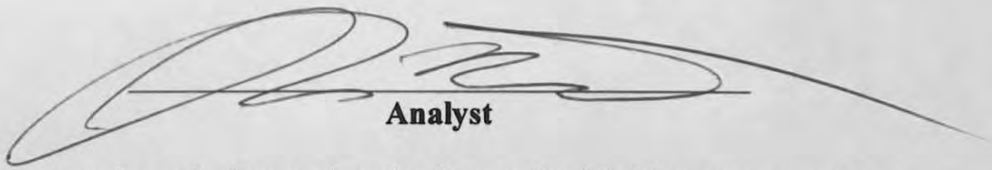

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Sampson Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008647 Clinton Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008647

Test Date: 02/12/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

06/08/2020-06/08/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002


Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	9:17pm
AIR BLK	.00	9:18pm
ACCY CHK	.08	9:18pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:20pm
AIR BLK	.00	9:21pm
SUB TEST	.00	9:22pm
AIR BLK	.00	9:23pm

Reported AC: .00 g/210L

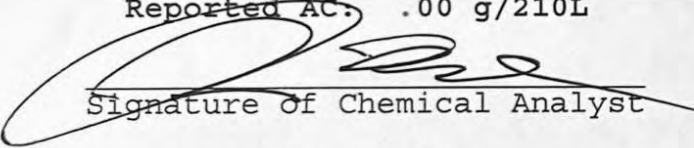
Signature of Chemical Analyst

Court CVR

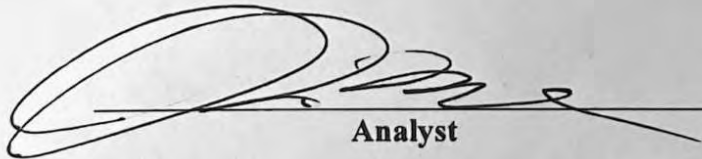
Analyst

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 5 810
Serial Number: 008647 Test Record Number: 2683
Test Date: 02/12/2022 Test Time: 9:24pm EST
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:24pm
FLO	Pass	9:24pm
FC	Pass	9:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:24pm
SRC	Pass	9:24pm
DET	Pass	9:24pm
BAR	Pass	9:24pm
BT	Pass	9:24pm

Blank Tests

Test	Status	Time
AIR	Pass	9:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:25pm

CRC Tests

Test	Status	Time
COMP	Pass	9:25pm
CAL	Pass	9:25pm

Preventive Maintenance
Status: Pass

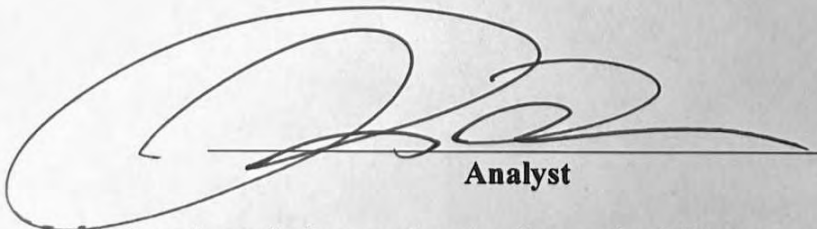

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Sampson Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008647 Clinton Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008647

Test Date: 02/12/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

06/08/2020-06/08/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002


Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	9:17pm
AIR BLK	.00	9:18pm
ACCY CHK	.08	9:18pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:20pm
AIR BLK	.00	9:21pm
SUB TEST	.00	9:22pm
AIR BLK	.00	9:23pm

Reported AC: .00 g/210L

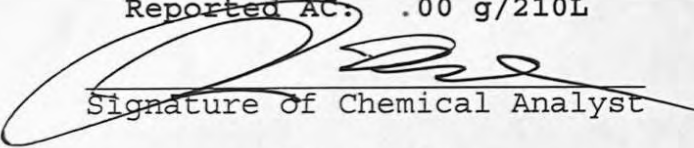
Signature of Chemical Analyst

Court CVR

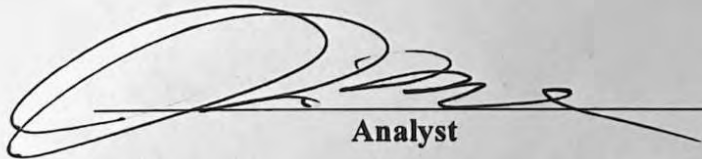
Analyst

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 5 810
Serial Number: 008647 Test Record Number: 2683
Test Date: 02/12/2022 Test Time: 9:24pm EST
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:24pm
FLO	Pass	9:24pm
FC	Pass	9:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:24pm
SRC	Pass	9:24pm
DET	Pass	9:24pm
BAR	Pass	9:24pm
BT	Pass	9:24pm

Blank Tests

Test	Status	Time
AIR	Pass	9:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:25pm

CRC Tests

Test	Status	Time
COMP	Pass	9:25pm
CAL	Pass	9:25pm

Preventive Maintenance
Status: Pass

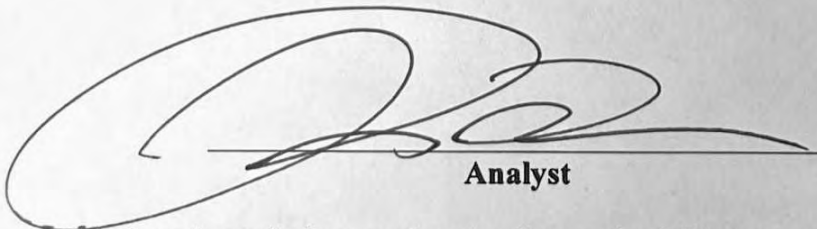

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location Locust PD
Instrument Serial No. 008706 Locust, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY LOCUST PD 830

Serial Number: 008706
Test Date: 02/09/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-

Effective:

00/00/0000-00/00/0000

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	11:23am
AIR BLK	.00	11:24am
ACCY CHK	.08	11:24am
AIR BLK	.00	11:25am
SUB TEST	.00	11:26am
AIR BLK	.00	11:27am
SUB TEST	.00	11:28am
AIR BLK	.00	11:29am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

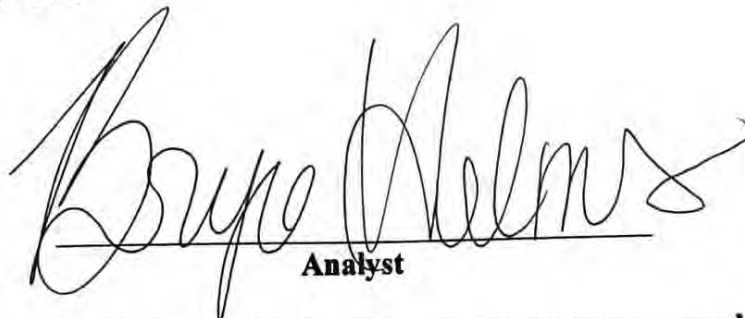

Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY LOCUST PD 830

Serial Number: 008706 Test Record Number: 3615
Test Date: 02/09/2022 Test Time: 11:30am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:30am
FLO	Pass	11:30am
FC	Pass	11:30am

Temperature Tests

Test	Status	Time
FC1	Pass	11:30am
SRC	Pass	11:30am
DET	Pass	11:30am
BAR	Pass	11:30am
BT	Pass	11:30am

Blank Tests

Test	Status	Time
AIR	Pass	11:31am


Printer Tests

Test	Status	Time
PRNT	Pass	11:31am

CRC Tests

Test	Status	Time
COMP	Pass	11:31am
CAL	Pass	11:31am

Preventive Maintenance
Status: *Pass*

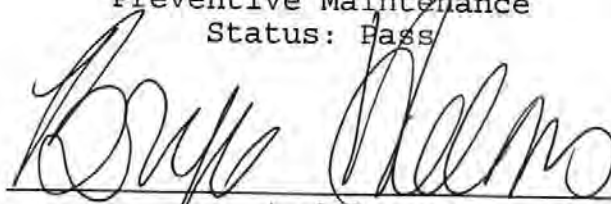

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location Stanly County 80
Instrument Serial No. 008847 Albemarle, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Adams
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842
Test Date: 02/23/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023


Test	g/210L	Time
DIAG	Pass	11:48am
AIR BLK	.00	11:49am
ACCY CHK	.08	11:50am
AIR BLK	.00	11:51am
SUB TEST	.00	11:52am
AIR BLK	.00	11:52am
SUB TEST	.00	11:54am
AIR BLK	.00	11:55am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

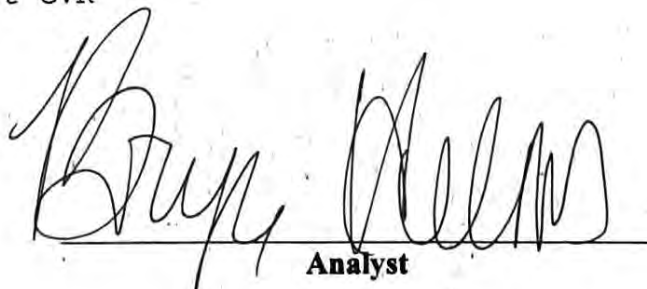
Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842 Test Record Number: 2518
Test Date: 02/23/2022 Test Time: 11:57am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:57am
FLO	Pass	11:57am
FC	Pass	11:57am

Temperature Tests

Test	Status	Time
FC1	Pass	11:57am
SRC	Pass	11:57am
DET	Pass	11:57am
BAR	Pass	11:57am
BT	Pass	11:57am

Blank Tests

Test	Status	Time
AIR	Pass	11:58am


Printer Tests

Test	Status	Time
PRNT	Pass	11:58am

CRC Tests

Test	Status	Time
COMP	Pass	11:58am
CAL	Pass	11:58am

Preventive Maintenance
Status: Pass

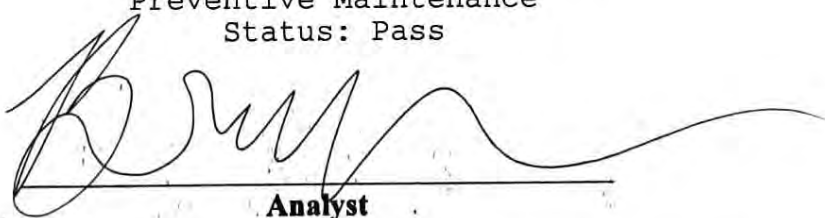

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location Stanly County 80
Instrument Serial No. 008927 Albemarle, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008927
Test Date: 02/23/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	11:56am
AIR BLK	.00	11:57am
ACCY CHK	.08	11:58am
AIR BLK	.00	11:59am
SUB TEST	.00	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:02pm
AIR BLK	.00	12:03pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008927 Test Record Number: 770
Test Date: 02/23/2022 Test Time: 12:03pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:03pm
FLO	Pass	12:03pm
FC	Pass	12:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:04pm
SRC	Pass	12:04pm
DET	Pass	12:04pm
BAR	Pass	12:04pm
BT	Pass	12:04pm

Blank Tests

Test	Status	Time
AIR	Pass	12:04pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:04pm

CRC Tests

Test	Status	Time
COMP	Pass	12:04pm
CAL	Pass	12:04pm

Preventive Maintenance
Status: Pass

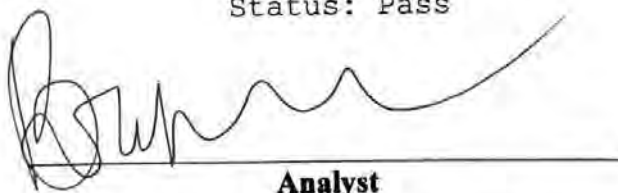

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Swain Instrument Location Swain Co Jail

Instrument Serial No. 008723 Boyson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Guth
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY JAIL 860

Serial Number: 008723

Test Date: 02/07/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401


Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	11:35am
AIR BLK	.00	11:35am
ACCY CHK	.08	11:36am
AIR BLK	.00	11:37am
SUB TEST	.00	11:38am
AIR BLK	.00	11:39am
SUB TEST	.00	11:40am
AIR BLK	.00	11:41am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

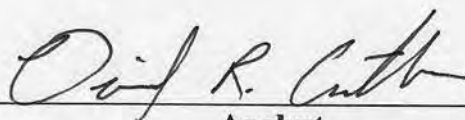

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY JAIL 860

Serial Number: 008723 Test Record Number: 845
Test Date: 02/07/2022 Test Time: 11:42am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:42am
FLO	Pass	11:42am
FC	Pass	11:42am

Temperature Tests

Test	Status	Time
FC1	Pass	11:42am
SRC	Pass	11:42am
DET	Pass	11:42am
BAR	Pass	11:42am
BT	Pass	11:42am

Blank Tests

Test	Status	Time
AIR	Pass	11:43am


Printer Tests

Test	Status	Time
PRNT	Pass	11:43am

CRC Tests

Test	Status	Time
COMP	Pass	11:43am
CAL	Pass	11:43am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Swain Instrument Location Swain Co Jail
Instrument Serial No. 008727 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Guth
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY JAIL 860

Serial Number: 008727

Test Date: 02/07/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401


Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	11:46am
AIR BLK	.00	11:47am
ACCY CHK	.08	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:49am
AIR BLK	.00	11:50am
SUB TEST	.00	11:51am
AIR BLK	.00	11:52am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY JAIL 860

Serial Number: 008727 Test Record Number: 1458
Test Date: 02/07/2022 Test Time: 11:53am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:53am
FLO	Pass	11:53am
FC	Pass	11:53am

Temperature Tests

Test	Status	Time
FC1	Pass	11:54am
SRC	Pass	11:54am
DET	Pass	11:54am
BAR	Pass	11:54am
BT	Pass	11:54am

Blank Tests

Test	Status	Time
AIR	Pass	11:54am


Printer Tests

Test	Status	Time
PRNT	Pass	11:54am

CRC Tests

Test	Status	Time
COMP	Pass	11:54am
CAL	Pass	11:54am

Preventive Maintenance
Status: Pass

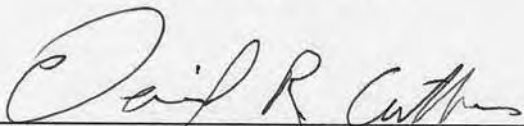

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Swain Instrument Location Cherokee Tribal Det
Instrument Serial No. 008782 Cherokee, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Cuth
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: 008782
Test Date: 02/08/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023


Test	g/210L	Time
DIAG	Pass	11:50am
AIR BLK	.00	11:50am
ACCY CHK	.07	11:51am
AIR BLK	.00	11:52am
SUB TEST	.00	11:53am
AIR BLK	.00	11:54am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: 008782 Test Record Number: 1315
Test Date: 02/08/2022 Test Time: 11:57am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:57am
FLO	Pass	11:57am
FC	Pass	11:57am

Temperature Tests

Test	Status	Time
FC1	Pass	11:58am
SRC	Pass	11:58am
DET	Pass	11:58am
BAR	Pass	11:58am
BT	Pass	11:58am

Blank Tests

Test	Status	Time
AIR	Pass	11:58am


Printer Tests

Test	Status	Time
PRNT	Pass	11:58am

CRC Tests

Test	Status	Time
COMP	Pass	11:58am
CAL	Pass	11:58am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Union County 80
Instrument Serial No. 0088666 Monroe, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008866
Test Date: 02/08/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Helms, Bryce A*
Permit Number: 0084-9845
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG035001
Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	11:36am
AIR BLK	.00	11:36am
ACCY CHK	.07	11:37am
AIR BLK	.00	11:38am
SUB TEST	.00	11:39am
AIR BLK	.00	11:40am
SUB TEST	.00	11:41am
AIR BLK	.00	11:42am

Reported AC: .00 g/210L

Bryce Helms

Signature of Chemical Analyst

Court CVR

Bryce Helms

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008866 Test Record Number: 3988
Test Date: 02/08/2022 Test Time: 11:43am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:44am
FLO	Pass	11:44am
FC	Pass	11:44am

Temperature Tests

Test	Status	Time
FC1	Pass	11:44am
SRC	Pass	11:44am
DET	Pass	11:44am
BAR	Pass	11:44am
BT	Pass	11:44am

Blank Tests

Test	Status	Time
AIR	Pass	11:44am


Printer Tests

Test	Status	Time
PRNT	Pass	11:45am

CRC Tests

Test	Status	Time
COMP	Pass	11:45am
CAL	Pass	11:45am

Preventive Maintenance
Status: *Pass*

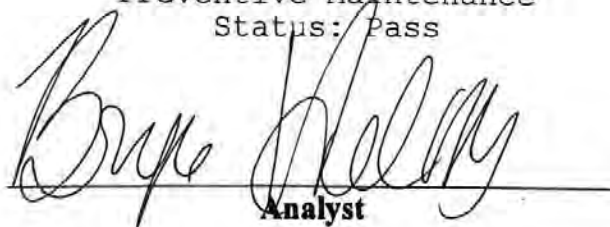
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Union Instrument Location Union County 80
Monroe, NC
Instrument Serial No. 008876

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 20 22 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

674

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008876
Test Date: 02/08/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018401
Exp Date: 07/02/2022


Test	g/210L	Time
DIAG	Pass	11:38am
AIR BLK	.00	11:38am
ACCY CHK	.07	11:39am
AIR BLK	.00	11:40am
SUB TEST	.00	11:41am
AIR BLK	.00	11:42am
SUB TEST	.00	11:44am
AIR BLK	.00	11:45am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

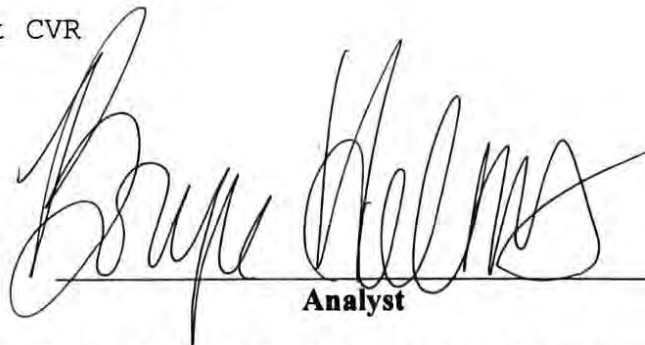

Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008876 Test Record Number: 6327
Test Date: 02/08/2022 Test Time: 11:45am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:46am
FLO	Pass	11:46am
FC	Pass	11:46am

Temperature Tests

Test	Status	Time
FC1	Pass	11:46am
SRC	Pass	11:46am
DET	Pass	11:46am
BAR	Pass	11:46am
BT	Pass	11:46am

Blank Tests

Test	Status	Time
AIR	Pass	11:46am


Printer Tests

Test	Status	Time
PRNT	Pass	11:46am

CRC Tests

Test	Status	Time
COMP	Pass	11:47am
CAL	Pass	11:47am

Preventive Maintenance
Status: *Pass*

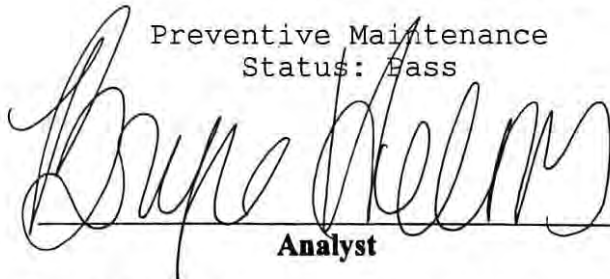

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Wake Co. Detention Center
3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

671

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577
Test Date: 02/28/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A
Permit Number: 0017-9707
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG202602
Exp Date: 01/26/2024


Test	g/210L	Time
DIAG	Pass	10:45am
AIR BLK	.00	10:46am
ACCY CHK	.07	10:47am
AIR BLK	.00	10:49am
SUB TEST	.00	10:49am
AIR BLK	.00	10:50am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577 Test Record Number: 6155
Test Date: 02/28/2022 Test Time: 10:58am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:58am
FLO	Pass	10:58am
FC	Pass	10:58am

Temperature Tests

Test	Status	Time
FC1	Pass	10:59am
SRC	Pass	10:59am
DET	Pass	10:59am
BAR	Pass	10:59am
BT	Pass	10:59am

Blank Tests

Test	Status	Time
AIR	Pass	10:59am

Printer Tests

Test	Status	Time
PRNT	Pass	10:59am

CRC Tests

Test	Status	Time
COMP	Pass	10:59am
CAL	Pass	10:59am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Wake Co. Detention Ctr
Instrument Serial No. 008612 3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008612
Test Date: 02/28/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG202602

Exp Date: 01/26/2024


Test	g/210L	Time
DIAG	Pass	10:46am
AIR BLK	.00	10:47am
ACCY CHK	.08	10:48am
AIR BLK	.00	10:49am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008612 Test Record Number: 4968
Test Date: 02/28/2022 Test Time: 10:59am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00am
FLO	Pass	11:00am
FC	Pass	11:00am

Temperature Tests

Test	Status	Time
FC1	Pass	11:00am
SRC	Pass	11:00am
DET	Pass	11:00am
BAR	Pass	11:00am
BT	Pass	11:00am

Blank Tests

Test	Status	Time
AIR	Pass	11:00am


Printer Tests

Test	Status	Time
PRNT	Pass	11:01am

CRC Tests

Test	Status	Time
COMP	Pass	11:01am
CAL	Pass	11:01am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Wake Co. Detention Ctr
Instrument Serial No. 008760 3301 Hammond RD
Raleigh NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760
Test Date: 02/28/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A
Permit Number: 0017-9707
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG202602
Exp Date: 01/26/2024

Test	g/210L	Time
DIAG	Pass	10:44am
AIR BLK	.00	10:45am
ACCY CHK	.08	10:45am
AIR BLK	.00	10:47am
SUB TEST	.00	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760 Test Record Number: 4782
Test Date: 02/28/2022 Test Time: 10:51am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:51am
FLO	Pass	10:51am
FC	Pass	10:51am

Temperature Tests

Test	Status	Time
FC1	Pass	10:52am
SRC	Pass	10:52am
DET	Pass	10:52am
BAR	Pass	10:52am
BT	Pass	10:52am

Blank Tests

Test	Status	Time
AIR	Pass	10:52am


Printer Tests

Test	Status	Time
PRNT	Pass	10:52am

CRC Tests

Test	Status	Time
COMP	Pass	10:52am
CAL	Pass	10:52am

Preventive Maintenance
Status: Pass

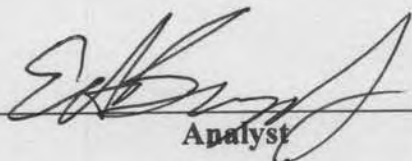

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake Co. Detention Center
Instrument Serial No. 008778 3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778
Test Date: 02/28/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG202602

Exp Date: 01/26/2024


Test	g/210L	Time
DIAG	Pass	10:45am
AIR BLK	.00	10:45am
ACCY CHK	.07	10:46am
AIR BLK	.00	10:47am
SUB TEST	.00	10:48am
AIR BLK	.00	10:49am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

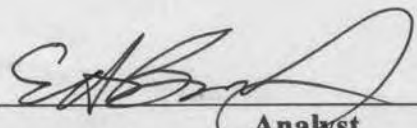

Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778 Test Record Number: 6675
Test Date: 02/28/2022 Test Time: 10:52am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52am
FLO	Pass	10:52am
FC	Pass	10:52am

Temperature Tests

Test	Status	Time
FC1	Pass	10:52am
SRC	Pass	10:52am
DET	Pass	10:52am
BAR	Pass	10:52am
BT	Pass	10:52am

Blank Tests

Test	Status	Time
AIR	Pass	10:53am


Printer Tests

Test	Status	Time
PRNT	Pass	10:53am

CRC Tests

Test	Status	Time
COMP	Pass	10:53am
CAL	Pass	10:53am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake Forest PD

Instrument Serial No. 008924 235 S Taylor St
Wake Forest, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of FEBRUARY, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

602

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY WAKE FOREST PD 910

Serial Number: 008924
Test Date: 02/14/2022

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2022-02/01/2024

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	11:57am
AIR BLK	.00	11:58am
ACCY CHK	.08	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:00pm
AIR BLK	.00	12:01pm
SUB TEST	.00	12:03pm
AIR BLK	.00	12:03pm

Reported AC: .00 g/210L

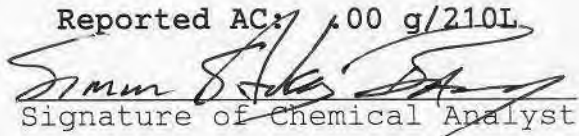
Signature of Chemical Analyst

Court CVR

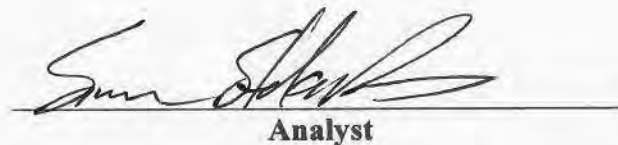
Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY WAKE FOREST PD 910

Serial Number: 008924 Test Record Number: 1647
Test Date: 02/14/2022 Test Time: 12:04pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:04pm
FLO	Pass	12:04pm
FC	Pass	12:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:05pm
SRC	Pass	12:05pm
DET	Pass	12:05pm
BAR	Pass	12:05pm
BT	Pass	12:05pm

Blank Tests

Test	Status	Time
AIR	Pass	12:05pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:05pm

CRC Tests

Test	Status	Time
COMP	Pass	12:05pm
CAL	Pass	12:05pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WARREN Instrument Location WARREN Co. LEC
Instrument Serial No. 008793 128 RAFTERS Lane
WARRENTON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008793

Test Date: 02/25/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501


Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	10:20am
AIR BLK	.00	10:21am
ACCY CHK	.07	10:21am
AIR BLK	.00	10:22am
SUB TEST	.00	10:23am
AIR BLK	.00	10:24am
SUB TEST	.00	10:25am
AIR BLK	.00	10:26am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008793 Test Record Number: 1839
Test Date: 02/25/2022 Test Time: 10:27am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:27am
FLO	Pass	10:27am
FC	Pass	10:27am

Temperature Tests

Test	Status	Time
FC1	Pass	10:27am
SRC	Pass	10:27am
DET	Pass	10:27am
BAR	Pass	10:27am
BT	Pass	10:27am

Blank Tests

Test	Status	Time
AIR	Pass	10:28am

Printer Tests

Test	Status	Time
PRNT	Pass	10:28am

CRC Tests

Test	Status	Time
COMP	Pass	10:28am
CAL	Pass	10:28am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Washington Instrument Location Washington Co. S.O.
Instrument Serial No. 008829 120 Adams St., Plymouth, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of January, 2012 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kim
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829
Test Date: 01/26/2022

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA


Agency: DHHS

Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	10:14am
AIR BLK	.00	10:15am
ACCY CHK	.07	10:16am
AIR BLK	.00	10:17am
SUB TEST	.00	10:18am
AIR BLK	.00	10:19am
SUB TEST	.00	10:20am
AIR BLK	.00	10:21am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829 Test Record Number: 1102
Test Date: 01/26/2022 Test Time: 10:22am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:22am
FLO	Pass	10:22am
FC	Pass	10:23am

Temperature Tests

Test	Status	Time
FC1	Pass	10:23am
SRC	Pass	10:23am
DET	Pass	10:23am
BAR	Pass	10:23am
BT	Pass	10:23am

Blank Tests

Test	Status	Time
AIR	Pass	10:23am


Printer Tests

Test	Status	Time
PRNT	Pass	10:23am

CRC Tests

Test	Status	Time
COMP	Pass	10:24am
CAL	Pass	10:24am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilkes Instrument Location Wilkes Co. Detention
Instrument Serial No. 008843 Wilkesboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

049
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008843
Test Date: 02/08/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	3:23pm
AIR BLK	.00	3:24pm
ACCY CHK	.08	3:25pm
AIR BLK	.00	3:26pm
SUB TEST	.00	3:26pm
AIR BLK	.00	3:27pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

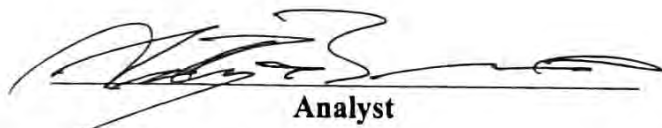
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008843 Test Record Number: 2628
Test Date: 02/08/2022 Test Time: 3:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:31pm
FLO	Pass	3:31pm
FC	Pass	3:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:31pm
SRC	Pass	3:31pm
DET	Pass	3:31pm
BAR	Pass	3:31pm
BT	Pass	3:31pm

Blank Tests

Test	Status	Time
AIR	Pass	3:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:32pm

CRC Tests

Test	Status	Time
COMP	Pass	3:32pm
CAL	Pass	3:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilkes Instrument Location Wilkes Co. Detention
Instrument Serial No. 008865 Wilkesboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2022 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008865

Test Date: 02/08/2022

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

02/01/2022-02/01/2024

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	3:23pm
AIR BLK	.00	3:24pm
ACCY CHK	.08	3:24pm
AIR BLK	.00	3:25pm
SUB TEST	.00	3:26pm
AIR BLK	.00	3:27pm
SUB TEST	.00	3:28pm
AIR BLK	.00	3:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008865 Test Record Number: 850
Test Date: 02/08/2022 Test Time: 3:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:30pm
FLO	Pass	3:30pm
FC	Pass	3:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:30pm
SRC	Pass	3:30pm
DET	Pass	3:30pm
BAR	Pass	3:30pm
BT	Pass	3:30pm

Blank Tests

Test	Status	Time
AIR	Pass	3:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:31pm

CRC Tests

Test	Status	Time
COMP	Pass	3:31pm
CAL	Pass	3:31pm

Preventive Maintenance
Status: Pass

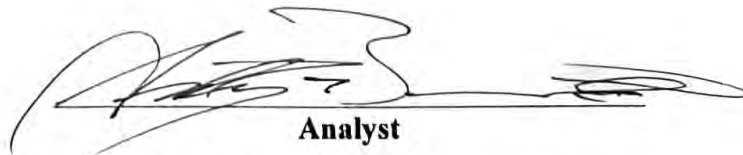

Analyst