

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 6
Instrument Serial No 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 6 000

Serial Number: 008779
Test Date: 12/17/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
09/01/2020-09/01/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG035001
Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	8:11pm
AIR BLK	.00	8:12pm
ACCY CHK	.07	8:12pm
AIR BLK	.00	8:13pm
SUB TEST	.00	8:13pm
AIR BLK	.00	8:14pm
SUB TEST	.00	8:16pm
AIR BLK	.00	8:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

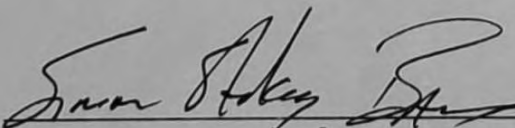
Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 6 000

Serial Number: 008779 Test Record Number: 3744
Test Date: 12/17/2021 Test Time: 8:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:20pm
FLO	Pass	8:20pm
FC	Pass	8:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:20pm
SRC	Pass	8:20pm
DET	Pass	8:20pm
BAR	Pass	8:20pm
BT	Pass	8:20pm

Blank Tests

Test	Status	Time
AIR	Pass	8:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:21pm

CRC Tests

Test	Status	Time
COMP	Pass	8:21pm
CAL	Pass	8:21pm

Preventive Maintenance
Status: Pass

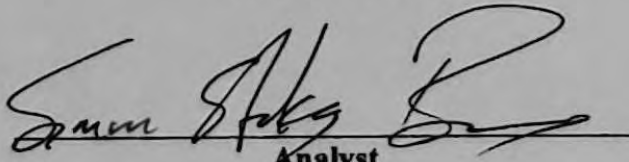
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alleghany Instrument Location Alleghany Co. Jail
Instrument Serial No. 008890 Spartan, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890
Test Date: 12/16/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	2:11pm
AIR BLK	.00	2:12pm
ACCY CHK	.07	2:12pm
AIR BLK	.00	2:13pm
SUB TEST	.00	2:14pm
AIR BLK	.00	2:15pm
SUB TEST	.00	2:16pm
AIR BLK	.00	2:17pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890 Test Record Number: 866
Test Date: 12/16/2021 Test Time: 2:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:18pm
FLO	Pass	2:18pm
FC	Pass	2:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:19pm
SRC	Pass	2:19pm
DET	Pass	2:19pm
BAR	Pass	2:19pm
BT	Pass	2:19pm

Blank Tests

Test	Status	Time
AIR	Pass	2:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:19pm

CRC Tests

Test	Status	Time
COMP	Pass	2:19pm
CAL	Pass	2:19pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Beaufort Instrument Location Beaufort Courthouse

Instrument Serial No. 008586 112 W. 2nd St., Washington, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586
Test Date: 12/14/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501


Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	1:25pm
AIR BLK	.00	1:25pm
ACCY CHK	.07	1:26pm
AIR BLK	.00	1:27pm
SUB TEST	.00	1:28pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:30pm
AIR BLK	.00	1:31pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586 Test Record Number: 1899
Test Date: 12/14/2021 Test Time: 1:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:39pm
FLO	Pass	1:39pm
FC	Pass	1:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:40pm
SRC	Pass	1:40pm
DET	Pass	1:40pm
BAR	Pass	1:40pm
BT	Pass	1:40pm

Blank Tests

Test	Status	Time
AIR	Pass	1:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:40pm

CRC Tests

Test	Status	Time
COMP	Pass	1:40pm
CAL	Pass	1:40pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Beaufort Instrument Location Beaufort Co Courthouse

Instrument Serial No. 008909 112 W. 2nd St Washington, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6043
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909

Test Date: 12/14/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:44pm
AIR BLK	.00	1:45pm
ACCY CHK	.07	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:47pm
AIR BLK	.00	1:48pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909 Test Record Number: 3682
Test Date: 12/14/2021 Test Time: 1:56pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:57pm
FLO	Pass	1:57pm
FC	Pass	1:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:57pm
SRC	Pass	1:57pm
DET	Pass	1:57pm
BAR	Pass	1:57pm
BT	Pass	1:57pm

Blank Tests

Test	Status	Time
AIR	Pass	1:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:58pm

CRC Tests

Test	Status	Time
COMP	Pass	1:58pm
CAL	Pass	1:58pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Bladen Instrument Location Bladen County
Instrument Serial No. 008818 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of December, 2021, the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008818
Test Date: 12/15/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:28pm
AIR BLK	.00	1:29pm
ACCY CHK	.07	1:30pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:32pm
AIR BLK	.00	1:33pm
SUB TEST	.00	1:34pm
AIR BLK	.00	1:35pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY DETENTION, CENTER 080

Serial Number: 008818 Test Record Number: 1892
Test Date: 12/15/2021 Test Time: 1:38pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:38pm
FLO	Pass	1:38pm
FC	Pass	1:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:38pm
SRC	Pass	1:38pm
DET	Pass	1:38pm
BAR	Pass	1:38pm
BT	Pass	1:38pm

Blank Tests

Test	Status	Time
AIR	Pass	1:39pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:39pm

CRC Tests

Test	Status	Time
COMP	Pass	1:39pm
CAL	Pass	1:39pm

Preventive Maintenance
Status: *Pass*

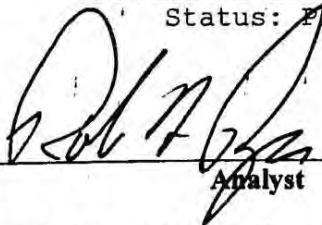

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Bladen Instrument Location Bladen County
Instrument Serial No. 008894 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008894
Test Date: 12/15/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:30pm
AIR BLK	.00	1:31pm
ACCY CHK	.08	1:31pm
AIR BLK	.00	1:33pm
SUB TEST	.00	1:33pm
AIR BLK	.00	1:34pm
SUB TEST	.00	1:36pm
AIR BLK	.00	1:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008894 Test Record Number: 1333
Test Date: 12/15/2021 Test Time: 1:38pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:38pm
FLO	Pass	1:38pm
FC	Pass	1:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:38pm
SRC	Pass	1:38pm
DET	Pass	1:38pm
BAR	Pass	1:38pm
BT	Pass	1:38pm

Blank Tests

Test	Status	Time
AIR	Pass	1:39pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:39pm

CRC Tests

Test	Status	Time
COMP	Pass	1:39pm
CAL	Pass	1:39pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location Brunswick County
Instrument Serial No. 008585 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008585
Test Date: 12/14/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	2:04pm
AIR BLK	.00	2:04pm
ACCY CHK	.07	2:05pm
AIR BLK	.00	2:06pm
SUB TEST	.00	2:07pm
AIR BLK	.00	2:07pm
SUB TEST	.00	2:09pm
AIR BLK	.00	2:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008585 Test Record Number: 4780
Test Date: 12/14/2021 Test Time: 2:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:12pm
FLO	Pass	2:12pm
FC	Pass	2:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:13pm
SRC	Pass	2:13pm
DET	Pass	2:13pm
BAR	Pass	2:13pm
BT	Pass	2:13pm

Blank Tests

Test	Status	Time
AIR	Pass	2:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:13pm

CRC Tests

Test	Status	Time
COMP	Pass	2:14pm
CAL	Pass	2:14pm

Preventive Maintenance
Status: *Pass*



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Brunswick Instrument Location Brunswick County
Instrument Serial No. 008602 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008602
Test Date: 12/14/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	1:48pm
AIR BLK	.00	1:49pm
ACCY CHK	.08	1:49pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:52pm
AIR BLK	.00	1:53pm
SUB TEST	.00	1:54pm
AIR BLK	.00	1:55pm

Reported to: .00 g/210L



Signature of Chemical Analyst

Court CVR

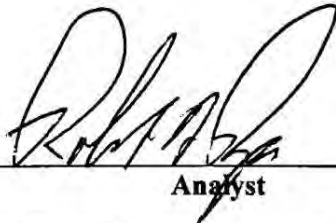

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008602 Test Record Number: 5015
Test Date: 12/14/2021 Test Time: 1:56pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:56pm
FLO	Pass	1:56pm
FC	Pass	1:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:57pm
SRC	Pass	1:57pm
DET	Pass	1:57pm
BAR	Pass	1:57pm
BT	Pass	1:57pm

Blank Tests

Test	Status	Time
AIR	Pass	1:57pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:57pm

CRC Tests

Test	Status	Time
COMP	Pass	1:57pm
CAL	Pass	1:57pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location Leland
Instrument Serial No. 008787 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY LELAND PD 090

Serial Number: 008787
Test Date: 12/06/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	10:01am
AIR BLK	.00	10:02am
ACCY CHK	.07	10:02am
AIR BLK	.00	10:03am
SUB TEST	.00	10:04am
AIR BLK	.00	10:05am
SUB TEST	.00	10:06am
AIR BLK	.00	10:07am

Reported AC/ .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY LELAND PD 090

Serial Number: 008787 Test Record Number: 944
Test Date: 12/06/2021 Test Time: 10:08am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:08am
FLO	Pass	10:08am
FC	Pass	10:08am

Temperature Tests

Test	Status	Time
FC1	Pass	10:08am
SRC	Pass	10:08am
DET	Pass	10:08am
BAR	Pass	10:08am
BT	Pass	10:08am

Blank Tests

Test	Status	Time
AIR	Pass	10:09am

Printer Tests

Test	Status	Time
PRNT	Pass	10:09am

CRC Tests

Test	Status	Time
COMP	Pass	10:09am
CAL	Pass	10:09am

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location Oak Island
Instrument Serial No. 008819 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY OAK ISLAND PD 090

Serial Number: 008819

Test Date: 12/10/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	3:20pm
AIR BLK	.00	3:21pm
ACCY CHK	.08	3:22pm
AIR BLK	.00	3:23pm
SUB TEST	.00	3:23pm
AIR BLK	.00	3:24pm
SUB TEST	.00	3:26pm
AIR BLK	.00	3:27pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY OAK ISLAND PD 090

Serial Number: 008819 Test Record Number: 841
Test Date: 12/10/2021 Test Time: 3:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:30pm
FLO	Pass	3:30pm
FC	Pass	3:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:30pm
SRC	Pass	3:30pm
DET	Pass	3:30pm
BAR	Pass	3:30pm
BT	Pass	3:30pm

Blank Tests

Test	Status	Time
AIR	Pass	3:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:31pm

CRC Tests

Test	Status	Time
COMP	Pass	3:31pm
CAL	Pass	3:31pm

Preventive Maintenance
Status: *Pass*

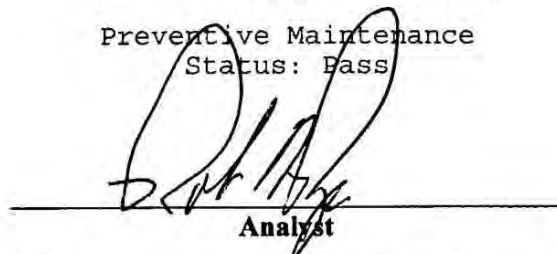

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location Sunset Beach
Instrument Serial No. 008874 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY SUNSET BEACH PD 090

Serial Number: 008874
Test Date: 12/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	1:46pm
AIR BLK	.00	1:46pm
ACCY CHK	.07	1:47pm
AIR BLK	.00	1:48pm
SUB TEST	.00	1:49pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:51pm
AIR BLK	.00	1:52pm

Reported AC: .00 g/210L

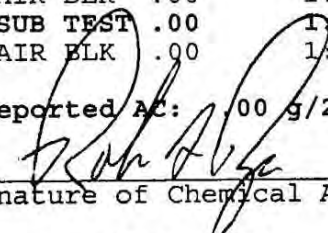

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY SUNSET BEACH PD 090

Serial Number: 008874 Test Record Number: 789
Test Date: 12/03/2021 Test Time: 1:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:53pm
FLO	Pass	1:53pm
FC	Pass	1:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:53pm
SRC	Pass	1:53pm
DET	Pass	1:53pm
BAR	Pass	1:53pm
BT	Pass	1:53pm

Blank Tests

Test	Status	Time
AIR	Pass	1:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:54pm

CRC Tests

Test	Status	Time
COMP	Pass	1:54pm
CAL	Pass	1:54pm

Preventive Maintenance
Status: *Pass*



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location Black Mountain Police Dept

Instrument Serial No. 009677 Black Mountain, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1068
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BLACK MOUNTAIN PD 100

Serial Number: 008697

Test Date: 12/29/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	10:01am
AIR BLK	.00	10:01am
ACCY CHK	.08	10:02am
AIR BLK	.00	10:03am
SUB TEST	.00	10:04am
AIR BLK	.00	10:04am
SUB TEST	.00	10:06am
AIR BLK	.00	10:07am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BLACK MOUNTAIN PD 100

Serial Number: 008697 Test Record Number: 4010
Test Date: 12/29/2021 Test Time: 10:07am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:07am
FLO	Pass	10:07am
FC	Pass	10:08am

Temperature Tests

Test	Status	Time
FC1	Pass	10:08am
SRC	Pass	10:08am
DET	Pass	10:08am
BAR	Pass	10:08am
BT	Pass	10:08am

Blank Tests

Test	Status	Time
AIR	Pass	10:08am

Printer Tests

Test	Status	Time
PRNT	Pass	10:08am

CRC Tests

Test	Status	Time
COMP	Pass	10:08am
CAL	Pass	10:08am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Burke Instrument Location Burke County Jail

Instrument Serial No. 008831 Morganton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008831
Test Date: 12/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	1:21pm
AIR BLK	.00	1:22pm
ACCY CHK	.08	1:22pm
AIR BLK	.00	1:24pm
SUB TEST	.00	1:24pm
AIR BLK	.00	1:25pm
SUB TEST	.00	1:27pm
AIR BLK	.00	1:27pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008831 Test Record Number: 2463
Test Date: 12/02/2021 Test Time: 1:28pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:28pm
FLO	Pass	1:28pm
FC	Pass	1:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:28pm
SRC	Pass	1:28pm
DET	Pass	1:28pm
BAR	Pass	1:28pm
BT	Pass	1:28pm

Blank Tests

Test	Status	Time
AIR	Pass	1:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:29pm

CRC Tests

Test	Status	Time
COMP	Pass	1:29pm
CAL	Pass	1:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Burke Instrument Location Burke County Jail

Instrument Serial No. 008907 Margerton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008904
Test Date: 12/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	1:18pm
AIR BLK	.00	1:19pm
ACCY CHK	.08	1:20pm
AIR BLK	.00	1:21pm
SUB TEST	.00	1:22pm
AIR BLK	.00	1:22pm
SUB TEST	.00	1:24pm
AIR BLK	.00	1:25pm

Reported AC: .00 g/210L



Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008904 Test Record Number: 2659
Test Date: 12/02/2021 Test Time: 1:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:26pm
FLO	Pass	1:26pm
FC	Pass	1:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:26pm
SRC	Pass	1:26pm
DET	Pass	1:26pm
BAR	Pass	1:26pm
BT	Pass	1:26pm

Blank Tests

Test	Status	Time
AIR	Pass	1:26pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:27pm

CRC Tests

Test	Status	Time
COMP	Pass	1:27pm
CAL	Pass	1:27pm

Preventive Maintenance
Status: Pass

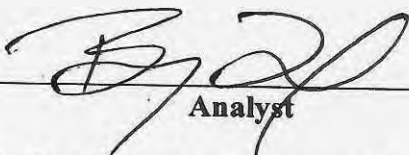

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caldwell Instrument Location Caldwell Co Jail
Instrument Serial No. 008803 Lenoir, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

049
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008803
Test Date: 12/20/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	2:51pm
AIR BLK	.00	2:52pm
ACCY CHK	.07	2:53pm
AIR BLK	.00	2:54pm
SUB TEST	.00	2:55pm
AIR BLK	.00	2:56pm
SUB TEST	.00	2:57pm
AIR BLK	.00	2:58pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008803 Test Record Number: 755
Test Date: 12/20/2021 Test Time: 2:59pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:00pm
FLO	Pass	3:00pm
FC	Pass	3:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:00pm
SRC	Pass	3:00pm
DET	Pass	3:00pm
BAR	Pass	3:00pm
BT	Pass	3:00pm

Blank Tests

Test	Status	Time
AIR	Pass	3:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:01pm

CRC Tests

Test	Status	Time
COMP	Pass	3:01pm
CAL	Pass	3:01pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caldwell Instrument Location Caldwell Co. Jail
Instrument Serial No. 008719 Lenoir, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008719
Test Date: 12/20/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Burnette, Anthony J
Permit Number: 0018-4401
Effective:
10/01/2020-10/01/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	2:52pm
AIR BLK	.00	2:53pm
ACCY CHK	.07	2:54pm
AIR BLK	.00	2:55pm
SUB TEST	.00	2:55pm
AIR BLK	.00	2:56pm
SUB TEST	.00	2:58pm
AIR BLK	.00	2:59pm

Reported AC: .00 g/210L

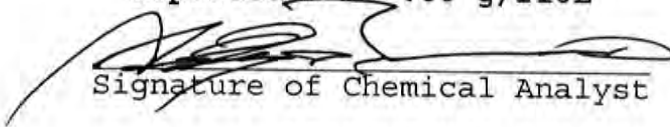

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008719 Test Record Number: 2927
Test Date: 12/20/2021 Test Time: 3:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:00pm
FLO	Pass	3:00pm
FC	Pass	3:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:00pm
SRC	Pass	3:00pm
DET	Pass	3:00pm
BAR	Pass	3:00pm
BT	Pass	3:00pm

Blank Tests

Test	Status	Time
AIR	Pass	3:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:01pm

CRC Tests

Test	Status	Time
COMP	Pass	3:01pm
CAL	Pass	3:01pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CARTERET Instrument Location CARTERET COUNTY
Instrument Serial No. 008605 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Ray Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008605
Test Date: 12/21/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	2:00pm
AIR BLK	.00	2:00pm
ACCY CHK	.08	2:01pm
AIR BLK	.00	2:02pm
SUB TEST	.00	2:03pm
AIR BLK	.00	2:04pm
SUB TEST	.00	2:05pm
AIR BLK	.00	2:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008605 Test Record Number: 4099
Test Date: 12/21/2021 Test Time: 2:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:08pm
FLO	Pass	2:08pm
FC	Pass	2:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:09pm
SRC	Pass	2:09pm
DET	Pass	2:09pm
BAR	Pass	2:09pm
BT	Pass	2:09pm

Blank Tests

Test	Status	Time
AIR	Pass	2:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:09pm

CRC Tests

Test	Status	Time
COMP	Pass	2:09pm
CAL	Pass	2:09pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CARTERET Instrument Location EMERALD ISLE
Instrument Serial No. 008620 POLICE DEPT.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008620
Test Date: 12/21/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG131901
Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	4:19pm
AIR BLK	.00	4:20pm
ACCY CHK	.08	4:21pm
AIR BLK	.00	4:22pm
SUB TEST	.00	4:23pm
AIR BLK	.00	4:24pm
SUB TEST	.00	4:25pm
AIR BLK	.00	4:26pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008620 Test Record Number: 2295
Test Date: 12/21/2021 Test Time: 4:27pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:27pm
FLO	Pass	4:27pm
FC	Pass	4:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:27pm
SRC	Pass	4:27pm
DET	Pass	4:27pm
BAR	Pass	4:27pm
BT	Pass	4:27pm

Blank Tests

Test	Status	Time
AIR	Pass	4:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:28pm

CRC Tests

Test	Status	Time
COMP	Pass	4:28pm
CAL	Pass	4:28pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CARTERET Instrument Location MOREHEAD CITY

Instrument Serial No. 008731 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Burns

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731
Test Date: 12/21/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG131901


Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	12:34pm
AIR BLK	.00	12:35pm
ACCY CHK	.08	12:36pm
AIR BLK	.00	12:37pm
SUB TEST	.00	12:37pm
AIR BLK	.00	12:38pm
SUB TEST	.00	12:40pm
AIR BLK	.00	12:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731 Test Record Number: 2400
Test Date: 12/21/2021 Test Time: 12:42pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:42pm
FLO	Pass	12:42pm
FC	Pass	12:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:42pm
SRC	Pass	12:42pm
DET	Pass	12:42pm
BAR	Pass	12:42pm
BT	Pass	12:42pm

Blank Tests

Test	Status	Time
AIR	Pass	12:43pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:43pm

CRC Tests

Test	Status	Time
COMP	Pass	12:43pm
CAL	Pass	12:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CARTERET Instrument Location ATLANTIC BEACH
Instrument Serial No. 008785 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Benson
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: 008785
Test Date: 12/21/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG131901
Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	10:59am
AIR BLK	.00	11:00am
ACCY CHK	.08	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:03am
AIR BLK	.00	11:04am
SUB TEST	.00	11:05am
AIR BLK	.00	11:06am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: 008785 Test Record Number: 1337
Test Date: 12/21/2021 Test Time: 11:07am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07am
FLO	Pass	11:07am
FC	Pass	11:07am

Temperature Tests

Test	Status	Time
FC1	Pass	11:07am
SRC	Pass	11:07am
DET	Pass	11:07am
BAR	Pass	11:07am
BT	Pass	11:07am

Blank Tests

Test	Status	Time
AIR	Pass	11:08am


Printer Tests

Test	Status	Time
PRNT	Pass	11:08am

CRC Tests

Test	Status	Time
COMP	Pass	11:08am
CAL	Pass	11:08am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CARTERET Instrument Location CARTERET COUNTY
Instrument Serial No. 008882 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alvin R. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008882
Test Date: 12/21/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	1:59pm
AIR BLK	.00	1:59pm
ACCY CHK	.08	2:00pm
AIR BLK	.00	2:01pm
SUB TEST	.00	2:02pm
AIR BLK	.00	2:03pm
SUB TEST	.00	2:04pm
AIR BLK	.00	2:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008882 Test Record Number: 2241
Test Date: 12/21/2021 Test Time: 2:05pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:06pm
FLO	Pass	2:06pm
FC	Pass	2:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:06pm
SRC	Pass	2:06pm
DET	Pass	2:06pm
BAR	Pass	2:06pm
BT	Pass	2:06pm

Blank Tests

Test	Status	Time
AIR	Pass	2:06pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:07pm

CRC Tests

Test	Status	Time
COMP	Pass	2:07pm
CAL	Pass	2:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Catawba Instrument Location Catawba Co SO

Instrument Serial No. 008687 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687
Test Date: 12/17/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	1:13pm
AIR BLK	.00	1:14pm
ACCY CHK	.08	1:15pm
AIR BLK	.00	1:17pm
SUB TEST	.00	1:18pm
AIR BLK	.00	1:19pm
SUB TEST	.00	1:21pm
AIR BLK	.00	1:22pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687 Test Record Number: 3381
Test Date: 12/17/2021 Test Time: 1:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:23pm
FLO	Pass	1:23pm
FC	Pass	1:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:23pm
SRC	Pass	1:23pm
DET	Pass	1:23pm
BAR	Pass	1:23pm
BT	Pass	1:23pm

Blank Tests

Test	Status	Time
AIR	Pass	1:24pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:24pm

CRC Tests

Test	Status	Time
COMP	Pass	1:24pm
CAL	Pass	1:24pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Catawba Instrument Location Catawba Co. 50
Instrument Serial No. 008821 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170.

Serial Number: 008821
Test Date: 12/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	1:14pm
AIR BLK	.00	1:14pm
ACCY CHK	.07	1:15pm
AIR BLK	.00	1:16pm
SUB TEST	.00	1:18pm
AIR BLK	.00	1:19pm
SUB TEST	.00	1:20pm
AIR BLK	.00	1:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821 Test Record Number: 2229
Test Date: 12/17/2021 Test Time: 1:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:26pm
FLO	Pass	1:26pm
FC	Pass	1:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:26pm
SRC	Pass	1:26pm
DET	Pass	1:26pm
BAR	Pass	1:26pm
BT	Pass	1:26pm

Blank Tests

Test	Status	Time
AIR	Pass	1:26pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:26pm

CRC Tests

Test	Status	Time
COMP	Pass	1:27pm
CAL	Pass	1:27pm

Preventive Maintenance
Status: Pass

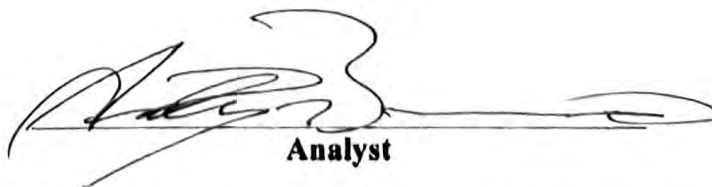

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Catawba Instrument Location Hickory Police Dept.
Instrument Serial No. 008841 Hickory, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

049
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841

Test Date: 12/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	2:21pm
AIR BLK	.00	2:22pm
ACCY CHK	.08	2:23pm
AIR BLK	.00	2:24pm
SUB TEST	.00	2:25pm
AIR BLK	.00	2:26pm
SUB TEST	.00	2:27pm
AIR BLK	.00	2:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841 Test Record Number: 2206
Test Date: 12/17/2021 Test Time: 2:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:30pm
FLO	Pass	2:30pm
FC	Pass	2:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:31pm
SRC	Pass	2:31pm
DET	Pass	2:31pm
BAR	Pass	2:31pm
BT	Pass	2:31pm

Blank Tests

Test	Status	Time
AIR	Pass	2:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:31pm

CRC Tests

Test	Status	Time
COMP	Pass	2:31pm
CAL	Pass	2:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Chatham Instrument Location Chatham County

Instrument Serial No. 008591 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008591
Test Date: 12/15/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
03/10/2021-03/10/2023

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	10:36am
AIR BLK	.00	10:37am
ACCY CHK	.08	10:37am
AIR BLK	.00	10:38am
SUB TEST	.00	10:39am
AIR BLK	.00	10:40am
SUB TEST	.00	10:42am
AIR BLK	.00	10:42am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

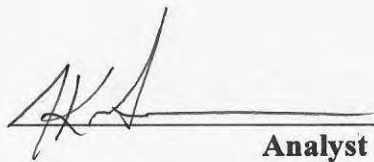

Analyst

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008591 Test Record Number: 2621
Test Date: 12/15/2021 Test Time: 10:43am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:44am
FLO	Pass	10:44am
FC	Pass	10:44am

Temperature Tests

Test	Status	Time
FC1	Pass	10:44am
SRC	Pass	10:44am
DET	Pass	10:44am
BAR	Pass	10:44am
BT	Pass	10:44am

Blank Tests

Test	Status	Time
AIR	Pass	10:44am


Printer Tests

Test	Status	Time
PRNT	Pass	10:44am

CRC Tests

Test	Status	Time
COMP	Pass	10:45am
CAL	Pass	10:45am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Chatham Instrument Location Siler City

Instrument Serial No. 008811 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY SILER CITY PD 180

Serial Number: 008811

Test Date: 12/15/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

03/10/2021-03/10/2023

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118803

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	11:36am
AIR BLK	.00	11:37am
ACCY CHK	.08	11:38am
AIR BLK	.00	11:39am
SUB TEST	.00	11:40am
AIR BLK	.00	11:41am
SUB TEST	.00	11:42am
AIR BLK	.00	11:43am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY SILER CITY PD 180

Serial Number: 008811 Test Record Number: 1527
Test Date: 12/15/2021 Test Time: 11:44am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:44am
FLO	Pass	11:44am
FC	Pass	11:44am

Temperature Tests

Test	Status	Time
FC1	Pass	11:45am
SRC	Pass	11:45am
DET	Pass	11:45am
BAR	Pass	11:45am
BT	Pass	11:45am

Blank Tests

Test	Status	Time
AIR	Pass	11:45am


Printer Tests

Test	Status	Time
PRNT	Pass	11:45am

CRC Tests

Test	Status	Time
COMP	Pass	11:45am
CAL	Pass	11:45am

Preventive Maintenance
Status: Pass

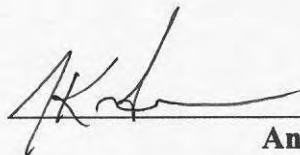

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cherokee Instrument Location Cherokee Co Jail

Instrument Serial No. 008622 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Guth
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: 008622
Test Date: 12/07/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	11:22am
AIR BLK	.00	11:23am
ACCY CHK	.07	11:24am
AIR BLK	.00	11:25am
SUB TEST	.00	11:26am
AIR BLK	.00	11:27am
SUB TEST	.00	11:28am
AIR BLK	.00	11:29am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: 008622 Test Record Number: 1175
Test Date: 12/07/2021 Test Time: 11:30am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:31am
FLO	Pass	11:31am
FC	Pass	11:31am

Temperature Tests

Test	Status	Time
FC1	Pass	11:31am
SRC	Pass	11:31am
DET	Pass	11:31am
BAR	Pass	11:31am
BT	Pass	11:31am

Blank Tests

Test	Status	Time
AIR	Pass	11:32am

Printer Tests

Test	Status	Time
PRNT	Pass	11:32am

CRC Tests

Test	Status	Time
COMP	Pass	11:32am
CAL	Pass	11:32am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cherokee Instrument Location Cherokee Co. Jail
Instrument Serial No. 008711 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: 008711
Test Date: 12/07/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	11:23am
AIR BLK	.00	11:24am
ACCY CHK	.07	11:25am
AIR BLK	.00	11:26am
SUB TEST	.00	11:27am
AIR BLK	.00	11:28am
SUB TEST	.00	11:30am
AIR BLK	.00	11:31am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: 008711 Test Record Number: 1158
Test Date: 12/07/2021 Test Time: 11:31am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:32am
FLO	Pass	11:32am
FC	Pass	11:32am

Temperature Tests

Test	Status	Time
FC1	Pass	11:32am
SRC	Pass	11:32am
DET	Pass	11:32am
BAR	Pass	11:32am
BT	Pass	11:32am

Blank Tests

Test	Status	Time
AIR	Pass	11:33am


Printer Tests

Test	Status	Time
PRNT	Pass	11:33am

CRC Tests

Test	Status	Time
COMP	Pass	11:33am
CAL	Pass	11:33am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Clay Instrument Location Clay County Jail
Instrument Serial No. 008608 Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Luth
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608
Test Date: 12/16/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:27am
AIR BLK	.00	10:28am
ACCY CHK	.08	10:28am
AIR BLK	.00	10:29am
SUB TEST	.00	10:30am
AIR BLK	.00	10:31am
SUB TEST	.00	10:33am
AIR BLK	.00	10:33am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608 Test Record Number: 1388
Test Date: 12/16/2021 Test Time: 10:34am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:34am
FLO	Pass	10:34am
FC	Pass	10:34am

Temperature Tests

Test	Status	Time
FC1	Pass	10:34am
SRC	Pass	10:34am
DET	Pass	10:34am
BAR	Pass	10:34am
BT	Pass	10:34am

Blank Tests

Test	Status	Time
AIR	Pass	10:35am

Printer Tests

Test	Status	Time
PRNT	Pass	10:35am

CRC Tests

Test	Status	Time
COMP	Pass	10:35am
CAL	Pass	10:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cleveland Instrument Location Cleveland Co. 50 - Annex

Instrument Serial No. 009997 Shelby, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1068
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008887
Test Date: 12/28/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	12:17pm
AIR BLK	.00	12:17pm
ACCY CHK	.07	12:18pm
AIR BLK	.00	12:19pm
SUB TEST	.00	12:20pm
AIR BLK	.00	12:21pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:23pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008887 Test Record Number: 3538
Test Date: 12/28/2021 Test Time: 12:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:26pm
FLO	Pass	12:26pm
FC	Pass	12:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:27pm
SRC	Pass	12:27pm
DET	Pass	12:27pm
BAR	Pass	12:27pm
BT	Pass	12:27pm

Blank Tests

Test	Status	Time
AIR	Pass	12:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:27pm

CRC Tests

Test	Status	Time
COMP	Pass	12:27pm
CAL	Pass	12:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cleveland Instrument Location Cleveland Co. 50 - Annex
Instrument Serial No. 007893 Shelby NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6068
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008893
Test Date: 12/28/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG132002
Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	12:16pm
AIR BLK	.00	12:17pm
ACCY CHK	.08	12:17pm
AIR BLK	.00	12:19pm
SUB TEST	.00	12:19pm
AIR BLK	.00	12:20pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:22pm

Reported AC: .00 g/210L

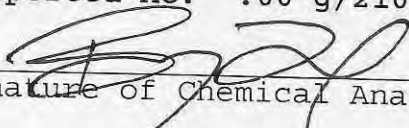

Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008893 Test Record Number: 1846
Test Date: 12/28/2021 Test Time: 12:23pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:23pm
FLO	Pass	12:23pm
FC	Pass	12:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:23pm
SRC	Pass	12:23pm
DET	Pass	12:23pm
BAR	Pass	12:23pm
BT	Pass	12:23pm

Blank Tests

Test	Status	Time
AIR	Pass	12:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:24pm

CRC Tests

Test	Status	Time
COMP	Pass	12:24pm
CAL	Pass	12:24pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cleveland Instrument Location King's Mountain Police Dept.

Instrument Serial No. 008900 King's Mountain, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900

Test Date: 12/28/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	10:51am
AIR BLK	.00	10:51am
ACCY CHK	.08	10:52am
AIR BLK	.00	10:53am
SUB TEST	.00	10:54am
AIR BLK	.00	10:55am
SUB TEST	.00	10:56am
AIR BLK	.00	10:57am

Reported AC: .00 g/210L

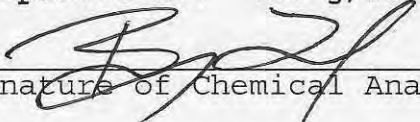

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900 Test Record Number: 896
Test Date: 12/28/2021 Test Time: 10:58am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:58am
FLO	Pass	10:58am
FC	Pass	10:58am

Temperature Tests

Test	Status	Time
FC1	Pass	10:58am
SRC	Pass	10:58am
DET	Pass	10:58am
BAR	Pass	10:58am
BT	Pass	10:58am

Blank Tests

Test	Status	Time
AIR	Pass	10:59am


Printer Tests

Test	Status	Time
PRNT	Pass	10:59am

CRC Tests

Test	Status	Time
COMP	Pass	10:59am
CAL	Pass	10:59am

Preventive Maintenance
Status: Pass

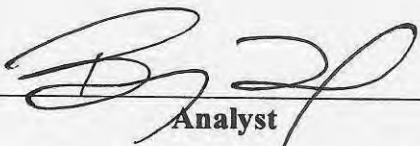

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location Columbus County
Instrument Serial No. 008875 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008875
Test Date: 12/15/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	3:45pm
AIR BLK	.00	3:45pm
ACCY CHK	.08	3:46pm
AIR BLK	.00	3:47pm
SUB TEST	.00	3:48pm
AIR BLK	.00	3:49pm
SUB TEST	.00	3:50pm
AIR BLK	.00	3:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008875 Test Record Number: 2568
Test Date: 12/15/2021 Test Time: 3:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:52pm
FLO	Pass	3:52pm
FC	Pass	3:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:52pm
SRC	Pass	3:52pm
DET	Pass	3:52pm
BAR	Pass	3:52pm
BT	Pass	3:52pm

Blank Tests

Test	Status	Time
AIR	Pass	3:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:53pm

CRC Tests

Test	Status	Time
COMP	Pass	3:53pm
CAL	Pass	3:53pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Columbus Instrument Location Tabor City

Instrument Serial No. 008886 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY TABOR CITY PD 230

Serial Number: 008886
Test Date: 12/15/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	4:44pm
AIR BLK	.00	4:45pm
ACCY CHK	.07	4:45pm
AIR BLK	.00	4:47pm
SUB TEST	.00	4:47pm
AIR BLK	.00	4:48pm
SUB TEST	.00	4:49pm
AIR BLK	.00	4:50pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY TABOR CITY PD 230

Serial Number: 008886 Test Record Number: 1613
Test Date: 12/15/2021 Test Time: 4:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:51pm
FLO	Pass	4:51pm
FC	Pass	4:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:51pm
SRC	Pass	4:51pm
DET	Pass	4:51pm
BAR	Pass	4:51pm
BT	Pass	4:51pm

Blank Tests

Test	Status	Time
AIR	Pass	4:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:52pm

CRC Tests

Test	Status	Time
COMP	Pass	4:52pm
CAL	Pass	4:52pm

Preventive Maintenance
Status: *Pass*

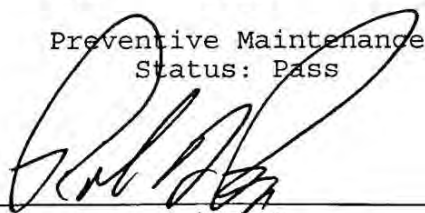

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Cumberland Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008575 Fayetteville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

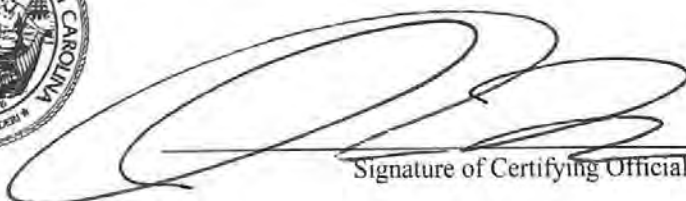


Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY BAT MOBILE UNIT 5
250

Serial Number: 008575
Test Date: 12/17/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Todd, Shane C
Permit Number: 0035-4789
Effective:
10/06/2020-10/06/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG118805
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	10:13pm
AIR BLK	.00	10:14pm
ACCY CHK	.08	10:15pm
AIR BLK	.00	10:16pm
SUB TEST	.00	10:16pm
AIR BLK	.00	10:17pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:20pm

Reported AC: .00 g/210L

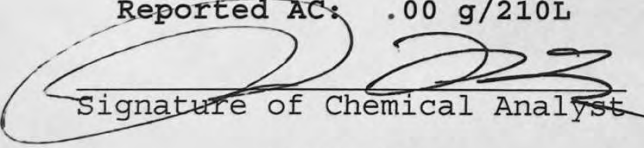
Signature of Chemical Analyst

Court CVR

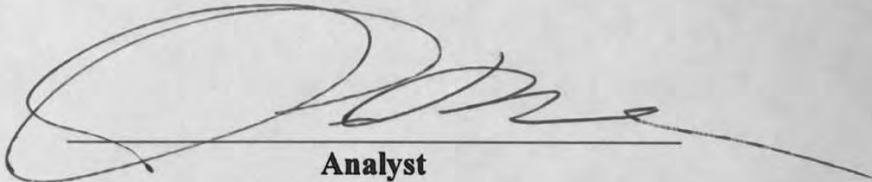
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY BAT MOBILE UNIT 5 250

Serial Number: 008575 Test Record Number: 1285
Test Date: 12/17/2021 Test Time: 10:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:22pm
FLO	Pass	10:22pm
FC	Pass	10:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:22pm
SRC	Pass	10:22pm
DET	Pass	10:22pm
BAR	Pass	10:22pm
BT	Pass	10:22pm

Blank Tests

Test	Status	Time
AIR	Pass	10:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:22pm

CRC Tests

Test	Status	Time
COMP	Pass	10:23pm
CAL	Pass	10:23pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cumberland Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008647 Fayetteville P.D.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY BAT MOBILE UNIT 5
250

Serial Number: 008647

Test Date: 12/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002


Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	10:17pm
AIR BLK	.00	10:18pm
ACCY CHK	.08	10:19pm
AIR BLK	.00	10:20pm
SUB TEST	.00	10:21pm
AIR BLK	.00	10:22pm
SUB TEST	.00	10:24pm
AIR BLK	.00	10:25pm

Reported AC: .00 g/210L

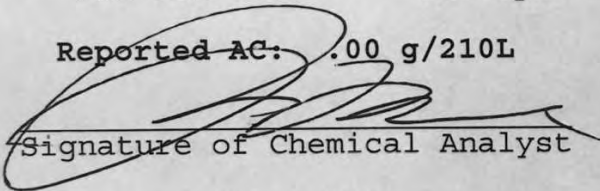
Signature of Chemical Analyst

Court CVR

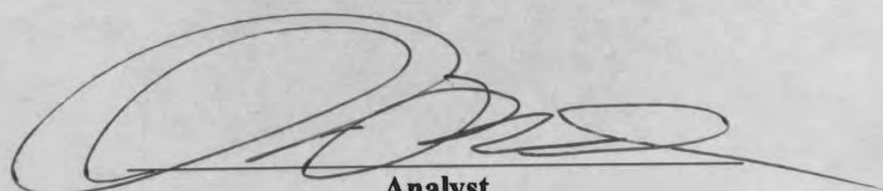
Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY BAT MOBILE UNIT 5 250
Serial Number: 008647 Test Record Number: 2671
Test Date: 12/17/2021 Test Time: 10:28pm EST
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:28pm
FLO	Pass	10:28pm
FC	Pass	10:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:28pm
SRC	Pass	10:28pm
DET	Pass	10:28pm
BAR	Pass	10:28pm
BT	Pass	10:28pm

Blank Tests

Test	Status	Time
AIR	Pass	10:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:29pm

CRC Tests

Test	Status	Time
COMP	Pass	10:29pm
CAL	Pass	10:29pm

Preventive Maintenance
Status: Pass

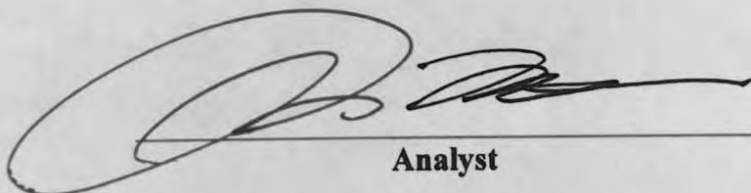

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Dare Instrument Location Kill Devil Hills P.D.

Instrument Serial No. 008844 107 Town Hall Dr, Kill Devil Hills NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kus
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844

Test Date: 12/21/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	11:32am
AIR BLK	.00	11:33am
ACCY CHK	.07	11:34am
AIR BLK	.00	11:35am
SUB TEST	.00	11:35am
AIR BLK	.00	11:36am
SUB TEST	.00	11:38am
AIR BLK	.00	11:39am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844 Test Record Number: 2713
Test Date: 12/21/2021 Test Time: 11:41am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:42am
FLO	Pass	11:42am
FC	Pass	11:42am

Temperature Tests

Test	Status	Time
FC1	Pass	11:42am
SRC	Pass	11:42am
DET	Pass	11:42am
BAR	Pass	11:42am
BT	Pass	11:42am

Blank Tests

Test	Status	Time
AIR	Pass	11:43am

Printer Tests

Test	Status	Time
PRNT	Pass	11:43am

CRC Tests

Test	Status	Time
COMP	Pass	11:43am
CAL	Pass	11:43am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT mobile Unit 4
Instrument Serial No. 008869 Davidson Co

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6600
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 1 280

Serial Number: 008869
Test Date: 12/31/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Smith, Jason R
Permit Number: 0024-7428
Effective:
09/29/2020-09/29/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	10:15pm
AIR BLK	.00	10:16pm
ACCY CHK	.08	10:17pm
AIR BLK	.00	10:17pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:19pm
SUB TEST	.00	10:21pm
AIR BLK	.00	10:22pm

Reported AC: .00 g/210L

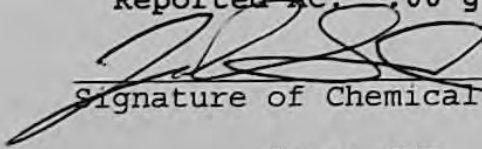
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 1 280

Serial Number: 008869 Test Record Number: 1221
Test Date: 12/31/2021 Test Time: 10:23pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:23pm
FLO	Pass	10:23pm
FC	Pass	10:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:23pm
SRC	Pass	10:23pm
DET	Pass	10:23pm
BAR	Pass	10:23pm
BT	Pass	10:23pm

Blank Tests

Test	Status	Time
AIR	Pass	10:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:24pm

CRC Tests

Test	Status	Time
COMP	Pass	10:24pm
CAL	Pass	10:24pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County DAVIDSON Instrument Location THOMASVILLE

Instrument Serial No. 008872 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16TH day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: 008872
Test Date: 12/16/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	1:00pm
AIR BLK	.00	1:01pm
ACCY CHK	.07	1:02pm
AIR BLK	.00	1:03pm
SUB TEST	.00	1:04pm
AIR BLK	.00	1:04pm
SUB TEST	.00	1:06pm
AIR BLK	.00	1:07pm

Reported AC: .00 g/210L

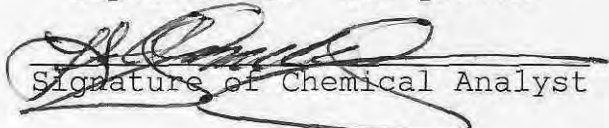
Signature of Chemical Analyst
Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: 008872 Test Record Number: 1579
Test Date: 12/16/2021 Test Time: 1:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:08pm
FLO	Pass	1:08pm
FC	Pass	1:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:08pm
SRC	Pass	1:08pm
DET	Pass	1:08pm
BAR	Pass	1:08pm
BT	Pass	1:08pm

Blank Tests

Test	Status	Time
AIR	Pass	1:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:09pm

CRC Tests

Test	Status	Time
COMP	Pass	1:09pm
CAL	Pass	1:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIE Instrument Location DAVIE COUNTY JAIL
Instrument Serial No. 008905 MOCKSVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22ND day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 669 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008905
Test Date: 12/22/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:28am
AIR BLK	.00	11:29am
ACCY CHK	.08	11:30am
AIR BLK	.00	11:31am
SUB TEST	.00	11:32am
AIR BLK	.00	11:33am
SUB TEST	.00	11:34am
AIR BLK	.00	11:35am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008905 Test Record Number: 2651
Test Date: 12/22/2021 Test Time: 11:36am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:36am
FLO	Pass	11:36am
FC	Pass	11:36am

Temperature Tests

Test	Status	Time
FC1	Pass	11:36am
SRC	Pass	11:36am
DET	Pass	11:36am
BAR	Pass	11:36am
BT	Pass	11:36am

Blank Tests

Test	Status	Time
AIR	Pass	11:37am

Printer Tests

Test	Status	Time
PRNT	Pass	11:37am

CRC Tests

Test	Status	Time
COMP	Pass	11:37am
CAL	Pass	11:37am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Durham Instrument Location BAT mobile Unit 6
Instrument Serial No. 008637 Durham

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY BAT MOBILE UNIT 6 310

Serial Number: 008637
Test Date: 12/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: *Varnell, Bryon L*

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: *Breath Test*

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	9:21pm
AIR BLK	.00	9:22pm
ACCY CHK	.07	9:22pm
AIR BLK	.00	9:23pm
SUB TEST	.00	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:26pm
AIR BLK	.00	9:27pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY BAT MOBILE UNIT 6 310

Serial Number: 008637 Test Record Number: 3174
Test Date: 12/03/2021 Test Time: 9:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:34pm
FLO	Pass	9:34pm
FC	Pass	9:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:34pm
SRC	Pass	9:34pm
DET	Pass	9:34pm
BAR	Pass	9:34pm
BT	Pass	9:34pm

Blank Tests

Test	Status	Time
AIR	Pass	9:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:35pm

CRC Tests

Test	Status	Time
COMP	Pass	9:35pm
CAL	Pass	9:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Durham Instrument Location BAT mobile unit 6

Instrument Serial No. 008686 Durham

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY BAT MOBILE UNIT 6 310

Serial Number: 008686

Test Date: 12/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	9:28pm
AIR BLK	.00	9:29pm
ACCY CHK	.07	9:30pm
AIR BLK	.00	9:31pm
SUB TEST	.00	9:31pm
AIR BLK	.00	9:32pm
SUB TEST	.00	9:33pm
AIR BLK	.00	9:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY BAT MOBILE UNIT 6 310

Serial Number: 008686 Test Record Number: 6814
Test Date: 12/03/2021 Test Time: 9:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:36pm
FLO	Pass	9:36pm
FC	Pass	9:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:36pm
SRC	Pass	9:36pm
DET	Pass	9:36pm
BAR	Pass	9:36pm
BT	Pass	9:36pm

Blank Tests

Test	Status	Time
AIR	Pass	9:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:37pm

CRC Tests

Test	Status	Time
COMP	Pass	9:37pm
CAL	Pass	9:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Durham Instrument Location BAT Mobile unit 6

Instrument Serial No. 008776 Durham

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY BAT MOBILE UNIT 6 310

Serial Number: 008776
Test Date: 12/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	9:16pm
AIR BLK	.00	9:17pm
ACCY CHK	.07	9:18pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:19pm
AIR BLK	.00	9:20pm
SUB TEST	.00	9:22pm
AIR BLK	.00	9:23pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY BAT MOBILE UNIT 6 310

Serial Number: 008776 Test Record Number: 3704
Test Date: 12/03/2021 Test Time: 9:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:33pm
FLO	Pass	9:33pm
FC	Pass	9:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:33pm
SRC	Pass	9:33pm
DET	Pass	9:33pm
BAR	Pass	9:33pm
BT	Pass	9:33pm

Blank Tests

Test	Status	Time
AIR	Pass	9:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:34pm

CRC Tests

Test	Status	Time
COMP	Pass	9:34pm
CAL	Pass	9:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location KERNERSVILLE
Instrument Serial No. 008650 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650
Test Date: 12/14/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG131901
Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	9:10am
AIR BLK	.00	9:11am
ACCY CHK	.08	9:12am
AIR BLK	.00	9:13am
SUB TEST	.00	9:13am
AIR BLK	.00	9:14am
SUB TEST	.00	9:16am
AIR BLK	.00	9:17am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650 Test Record Number: 1905
Test Date: 12/14/2021 Test Time: 9:18am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:18am
FLO	Pass	9:18am
FC	Pass	9:18am

Temperature Tests

Test	Status	Time
FC1	Pass	9:18am
SRC	Pass	9:18am
DET	Pass	9:18am
BAR	Pass	9:18am
BT	Pass	9:18am

Blank Tests

Test	Status	Time
AIR	Pass	9:19am

Printer Tests

Test	Status	Time
PRNT	Pass	9:19am

CRC Tests

Test	Status	Time
COMP	Pass	9:19am
CAL	Pass	9:19am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location FORSYTH CO. DETENTION

Instrument Serial No. 008896 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22ND day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008896
Test Date: 12/22/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118803
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	9:40am
AIR BLK	.00	9:41am
ACCY CHK	.07	9:42am
AIR BLK	.00	9:43am
SUB TEST	.00	9:45am
AIR BLK	.00	9:46am
SUB TEST	.00	9:48am
AIR BLK	.00	9:48am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008896 Test Record Number: 1481
Test Date: 12/22/2021 Test Time: 9:49am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:50am
FLO	Pass	9:50am
FC	Pass	9:50am

Temperature Tests

Test	Status	Time
FC1	Pass	9:50am
SRC	Pass	9:50am
DET	Pass	9:50am
BAR	Pass	9:50am
BT	Pass	9:50am

Blank Tests

Test	Status	Time
AIR	Pass	9:51am

Printer Tests

Test	Status	Time
PRNT	Pass	9:51am

CRC Tests

Test	Status	Time
COMP	Pass	9:51am
CAL	Pass	9:51am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location KERNERSVILLE
Instrument Serial No. 008896 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2ND day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008896
Test Date: 12/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Oligmueller Jr., Leo A*
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG131901
Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	1:47pm
AIR BLK	.00	1:48pm
ACCY CHK	.07	1:48pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:53pm
AIR BLK	.00	1:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008896 Test Record Number: 1473
Test Date: 12/02/2021 Test Time: 1:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:54pm
FLO	Pass	1:54pm
FC	Pass	1:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:55pm

CRC Tests

Test	Status	Time
COMP	Pass	1:55pm
CAL	Pass	1:55pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Gaston County 80
Instrument Serial No. 008643 Gaston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008643
Test Date: 12/16/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
04/20/2021-04/20/2023

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG132002
Exp Date: 11/16/2023


Test	g/210L	Time
DIAG	Pass	12:45pm
AIR BLK	.00	12:45pm
ACCY CHK	.07	12:46pm
AIR BLK	.00	12:47pm
SUB TEST	.00	12:48pm
AIR BLK	.00	12:49pm
SUB TEST	.00	12:50pm
AIR BLK	.00	12:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

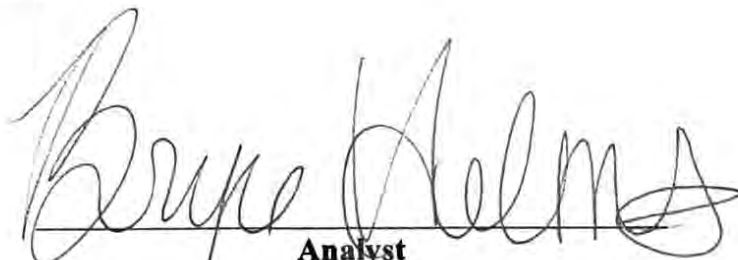

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008643 Test Record Number: 3825
Test Date: 12/16/2021 Test Time: 12:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:52pm
FLO	Pass	12:52pm
FC	Pass	12:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:53pm
SRC	Pass	12:53pm
DET	Pass	12:53pm
BAR	Pass	12:53pm
BT	Pass	12:53pm

Blank Tests

Test	Status	Time
AIR	Pass	12:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:53pm

CRC Tests

Test	Status	Time
COMP	Pass	12:53pm
CAL	Pass	12:53pm

Preventive Maintenance
Status: Pass

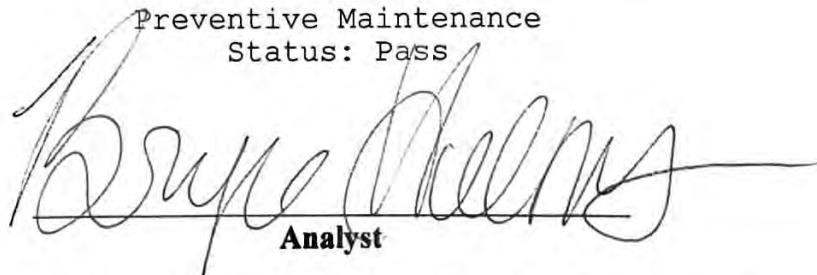

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Gaston County 80
Instrument Serial No. 008684 Gaston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008684
Test Date: 12/16/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG132002

Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	12:52pm
AIR BLK	.00	12:52pm
ACCY CHK	.08	12:53pm
AIR BLK	.00	12:54pm
SUB TEST	.00	12:55pm
AIR BLK	.00	12:55pm
SUB TEST	.00	12:57pm
AIR BLK	.00	12:58pm

Reported AC: .00 g/210L

Bryce Helms

Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008684 Test Record Number: 5366
Test Date: 12/16/2021 Test Time: 12:58pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:59pm
FLO	Pass	12:59pm
FC	Pass	12:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:59pm
SRC	Pass	12:59pm
DET	Pass	12:59pm
BAR	Pass	12:59pm
BT	Pass	12:59pm

Blank Tests

Test	Status	Time
AIR	Pass	12:59pm

Printer Tests


Test	Status	Time
PRNT	Pass	12:59pm

CRC Tests

Test	Status	Time
COMP	Pass	1:00pm
CAL	Pass	1:00pm

Preventive Maintenance

Status: Pass

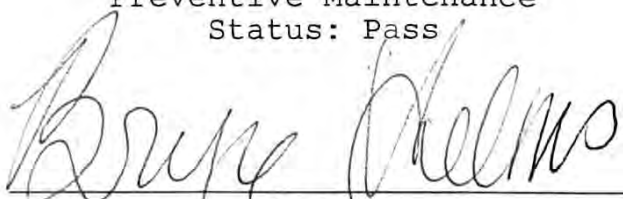

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Mt. Holly P.D
Instrument Serial No. 008733 Mt. Holly, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY MT. HOLLY PD 350

Serial Number: 008733

Test Date: 12/16/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	1:44pm
AIR BLK	.00	1:45pm
ACCY CHK	.07	1:45pm
AIR BLK	.00	1:46pm
SUB TEST	.00	1:47pm
AIR BLK	.00	1:48pm
SUB TEST	.00	1:49pm
AIR BLK	.00	1:50pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY MT. HOLLY PD 350

Serial Number: 008733 Test Record Number: 1285
Test Date: 12/16/2021 Test Time: 1:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:51pm
FLO	Pass	1:51pm
FC	Pass	1:51pm

Temperature Tests

Test	Status	Time
FCL	Pass	1:51pm
SRC	Pass	1:51pm
DET	Pass	1:51pm
BAR	Pass	1:51pm
BT	Pass	1:51pm

Blank Tests

Test	Status	Time
AIR	Pass	1:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:52pm

CRC Tests

Test	Status	Time
COMP	Pass	1:52pm
CAL	Pass	1:52pm

Preventive Maintenance
Status: Pass

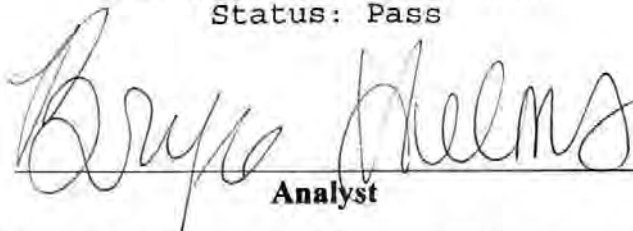
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Graham Instrument Location Graham Co. SO
Instrument Serial No. 008915 Robbinsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GRAHAM COUNTY GRAHAM COUNTY SD 370

Serial Number: 008915
Test Date: 12/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Cutler, Daniel R*
Permit Number: 0084-3310
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG007601
Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	10:25am
AIR BLK	.00	10:26am
ACCY CHK	.08	10:27am
AIR BLK	.00	10:28am
SUB TEST	.00	10:29am
AIR BLK	.00	10:30am
SUB TEST	.00	10:31am
AIR BLK	.00	10:32am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GRAHAM COUNTY GRAHAM COUNTY SD 370

Serial Number: 008915 Test Record Number: 856
Test Date: 12/02/2021 Test Time: 10:33am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:34am
FLO	Pass	10:34am
FC	Pass	10:34am

Temperature Tests

Test	Status	Time
FC1	Pass	10:34am
SRC	Pass	10:34am
DET	Pass	10:34am
BAR	Pass	10:34am
BT	Pass	10:34am

Blank Tests

Test	Status	Time
AIR	Pass	10:35am


Printer Tests

Test	Status	Time
PRNT	Pass	10:35am

CRC Tests

Test	Status	Time
COMP	Pass	10:35am
CAL	Pass	10:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Guilford Instrument Location Gibsonville PD

Instrument Serial No. 008812 129 W. Main St Gibsonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GIBSONVILLE PD 400

Serial Number: 008812

Test Date: 12/07/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

09/01/2020-09/01/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	2:28pm
AIR BLK	.00	2:29pm
ACCY CHK	.08	2:30pm
AIR BLK	.00	2:31pm
SUB TEST	.00	2:31pm
AIR BLK	.00	2:32pm
SUB TEST	.00	2:34pm
AIR BLK	.00	2:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GIBSONVILLE PD 400

Serial Number: 008812 Test Record Number: 3581
Test Date: 12/07/2021 Test Time: 2:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:35pm
FLO	Pass	2:35pm
FC	Pass	2:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:36pm
SRC	Pass	2:36pm
DET	Pass	2:36pm
BAR	Pass	2:36pm
BT	Pass	2:36pm

Blank Tests

Test	Status	Time
AIR	Pass	2:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:36pm

CRC Tests

Test	Status	Time
COMP	Pass	2:37pm
CAL	Pass	2:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 1
Instrument Serial No. 008869 Greensboro PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 1 400

Serial Number: 008869
Test Date: 12/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Smith, Jason R
Permit Number: 0024-7428
Effective:
09/29/2020-09/29/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	11:04pm
AIR BLK	.00	11:05pm
ACCY CHK	.07	11:05pm
AIR BLK	.00	11:06pm
SUB TEST	.00	11:07pm
AIR BLK	.00	11:08pm
SUB TEST	.00	11:10pm
AIR BLK	.00	11:11pm

Reported AC: .00 g/210L

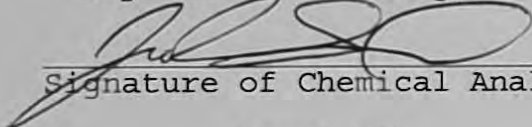

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 1 400

Serial Number: 008869 Test Record Number: 1218
Test Date: 12/03/2021 Test Time: 11:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:32pm
FLO	Pass	11:32pm
FC	Pass	11:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:32pm
SRC	Pass	11:32pm
DET	Pass	11:32pm
BAR	Pass	11:32pm
BT	Pass	11:32pm

Blank Tests

Test	Status	Time
AIR	Pass	11:33pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:33pm

CRC Tests

Test	Status	Time
COMP	Pass	11:33pm
CAL	Pass	11:33pm

Preventive Maintenance
Status: Pass

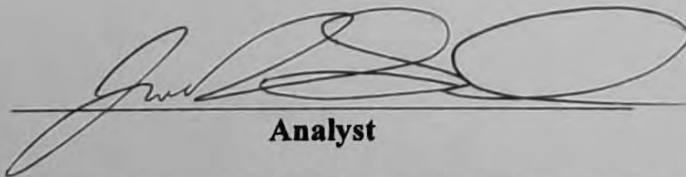

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 1

Instrument Serial No. 0001848 Greensboro

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 1 400

Serial Number: 008898
Test Date: 12/03/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Smith, Jason R

Permit Number: 0024-7428

Effective:

09/29/2020-09/29/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	11:10pm
AIR BLK	.00	11:11pm
ACCY CHK	.07	11:12pm
AIR BLK	.00	11:13pm
SUB TEST	.00	11:13pm
AIR BLK	.00	11:14pm
SUB TEST	.00	11:16pm
AIR BLK	.00	11:17pm

Reported AC: 00 g/210L

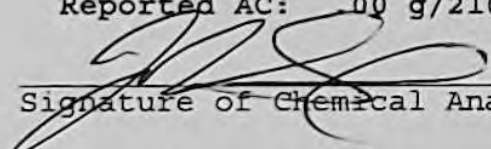

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 1 400

Serial Number: 008898 Test Record Number: 1241
Test Date: 12/03/2021 Test Time: 11:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:30pm
FLO	Pass	11:30pm
FC	Pass	11:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:30pm
SRC	Pass	11:30pm
DET	Pass	11:30pm
BAR	Pass	11:30pm
BT	Pass	11:30pm

Blank Tests

Test	Status	Time
AIR	Pass	11:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:31pm

CRC Tests

Test	Status	Time
COMP	Pass	11:31pm
CAL	Pass	11:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Haywood Instrument Location Haywood County Jail

Instrument Serial No. 008712 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008712

Test Date: 12/06/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	10:11am
AIR BLK	.00	10:12am
ACCY CHK	.08	10:13am
AIR BLK	.00	10:14am
SUB TEST	.00	10:15am
AIR BLK	.00	10:15am
SUB TEST	.00	10:17am
AIR BLK	.00	10:18am

Reported AC: .00 g/210L

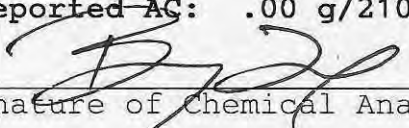
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008712 Test Record Number: 2437
Test Date: 12/06/2021 Test Time: 10:18am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:19am
FLO	Pass	10:19am
FC	Pass	10:19am

Temperature Tests

Test	Status	Time
FC1	Pass	10:19am
SRC	Pass	10:19am
DET	Pass	10:19am
BAR	Pass	10:19am
BT	Pass	10:19am

Blank Tests

Test	Status	Time
AIR	Pass	10:20am

Printer Tests

Test	Status	Time
PRNT	Pass	10:20am

CRC Tests

Test	Status	Time
COMP	Pass	10:20am
CAL	Pass	10:20am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Haywood Instrument Location Haywood County Jail

Instrument Serial No. 008714 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008714
Test Date: 12/06/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	10:09am
AIR BLK	.00	10:10am
ACCY CHK	.07	10:11am
AIR BLK	.00	10:12am
SUB TEST	.00	10:13am
AIR BLK	.00	10:14am
SUB TEST	.00	10:15am
AIR BLK	.00	10:16am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008714 Test Record Number: 1801
Test Date: 12/06/2021 Test Time: 10:17am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:17am
FLO	Pass	10:17am
FC	Pass	10:17am

Temperature Tests

Test	Status	Time
FC1	Pass	10:17am
SRC	Pass	10:17am
DET	Pass	10:17am
BAR	Pass	10:17am
BT	Pass	10:17am

Blank Tests

Test	Status	Time
AIR	Pass	10:18am

Printer Tests

Test	Status	Time
PRNT	Pass	10:18am

CRC Tests

Test	Status	Time
COMP	Pass	10:18am
CAL	Pass	10:18am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Haywood Instrument Location BAT MOBILE UNIT 2

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

673
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD BAT MOBILE UNIT 2 430

Serial Number: 008973

Test Date: 12/04/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barrier II, Dennis J

Permit Number: 0014-7953

Effective:

09/21/2020-09/21/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601


Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	8:38pm
AIR BLK	.00	8:39pm
ACCY CHK	.08	8:39pm
AIR BLK	.00	8:40pm
SUB TEST	.00	8:40pm
AIR BLK	.00	8:41pm
SUB TEST	.00	8:43pm
AIR BLK	.00	8:44pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

HAYWOOD BAT MOBILE UNIT 2 430

Serial Number: 008973 Test Record Number: 928
Test Date: 12/04/2021 Test Time: 8:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:45pm
FLO	Pass	8:45pm
FC	Pass	8:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:45pm
SRC	Pass	8:45pm
DET	Pass	8:45pm
BAR	Pass	8:45pm
BT	Pass	8:45pm

Blank Tests

Test	Status	Time
AIR	Pass	8:46pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:46pm

CRC Tests

Test	Status	Time
COMP	Pass	8:46pm
CAL	Pass	8:46pm

Preventive Maintenance
Status: Pass

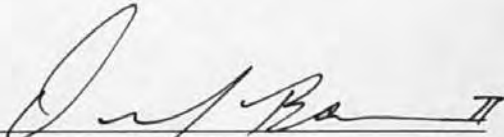

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hertford Instrument Location Aboskie P.D.
Instrument Serial No. 008848 705 W. Main St, Aboskie, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kun Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848
Test Date: 12/13/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Guard, Kelly G
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:46am
AIR BLK	.00	10:46am
ACCY CHK	.07	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:49am
AIR BLK	.00	10:50am
SUB TEST	.00	10:51am
AIR BLK	.00	10:52am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848 Test Record Number: 1659
Test Date: 12/13/2021 Test Time: 10:54am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:54am
FLO	Pass	10:54am
FC	Pass	10:54am

Temperature Tests

Test	Status	Time
FC1	Pass	10:54am
SRC	Pass	10:54am
DET	Pass	10:54am
BAR	Pass	10:54am
BT	Pass	10:54am

Blank Tests

Test	Status	Time
AIR	Pass	10:55am

Printer Tests

Test	Status	Time
PRNT	Pass	10:55am

CRC Tests

Test	Status	Time
COMP	Pass	10:55am
CAL	Pass	10:55am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hertford Instrument Location Mt. Freshwater P.D.
Instrument Serial No. 009906 115 E. Road St, Mount Freshwater, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6113
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906

Test Date: 12/13/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:59pm
AIR BLK	.00	1:00pm
ACCY CHK	.08	1:00pm
AIR BLK	.00	1:01pm
SUB TEST	.00	1:02pm
AIR BLK	.00	1:03pm
SUB TEST	.00	1:05pm
AIR BLK	.00	1:05pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906 Test Record Number: 827
Test Date: 12/13/2021 Test Time: 1:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:07pm
FLO	Pass	1:07pm
FC	Pass	1:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:07pm
SRC	Pass	1:07pm
DET	Pass	1:07pm
BAR	Pass	1:07pm
BT	Pass	1:07pm

Blank Tests

Test	Status	Time
AIR	Pass	1:07pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:07pm

CRC Tests

Test	Status	Time
COMP	Pass	1:08pm
CAL	Pass	1:08pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Iredell Instrument Location Mooreville, PD

Instrument Serial No. 008685 Mooreville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685
Test Date: 12/01/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	2:08pm
AIR BLK	.00	2:09pm
ACCY CHK	.08	2:09pm
AIR BLK	.00	2:11pm
SUB TEST	.00	2:11pm
AIR BLK	.00	2:12pm
SUB TEST	.00	2:14pm
AIR BLK	.00	2:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685 Test Record Number: 3792
Test Date: 12/01/2021 Test Time: 2:15pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:15pm
FLO	Pass	2:15pm
FC	Pass	2:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:15pm
SRC	Pass	2:15pm
DET	Pass	2:15pm
BAR	Pass	2:15pm
BT	Pass	2:15pm

Blank Tests

Test	Status	Time
AIR	Pass	2:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:16pm

CRC Tests

Test	Status	Time
COMP	Pass	2:16pm
CAL	Pass	2:16pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Jackson Instrument Location Jackson County Jail
Instrument Serial No. 008708 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 635 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008708
Test Date: 12/09/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	10:15am
AIR BLK	.00	10:16am
ACCY CHK	.07	10:17am
AIR BLK	.00	10:17am
SUB TEST	.00	10:18am
AIR BLK	.00	10:19am
SUB TEST	.00	10:20am
AIR BLK	.00	10:21am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008708 Test Record Number: 1615
Test Date: 12/09/2021 Test Time: 10:22am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:22am
FLO	Pass	10:22am
FC	Pass	10:22am

Temperature Tests

Test	Status	Time
FC1	Pass	10:22am
SRC	Pass	10:22am
DET	Pass	10:22am
BAR	Pass	10:22am
BT	Pass	10:22am

Blank Tests

Test	Status	Time
AIR	Pass	10:23am


Printer Tests

Test	Status	Time
PRNT	Pass	10:23am

CRC Tests

Test	Status	Time
COMP	Pass	10:23am
CAL	Pass	10:23am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Jackson Instrument Location Jackson County Jail
Instrument Serial No. 608722 Sylvan, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Guth

Signature of Certifying Official

635

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008722

Test Date: 12/09/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401


Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	10:16am
AIR BLK	.00	10:17am
ACCY CHK	.07	10:17am
AIR BLK	.00	10:19am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am
SUB TEST	.00	10:21am
AIR BLK	.00	10:22am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008722 Test Record Number: 1296
Test Date: 12/09/2021 Test Time: 10:23am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:23am
FLO	Pass	10:23am
FC	Pass	10:23am

Temperature Tests

Test	Status	Time
FC1	Pass	10:23am
SRC	Pass	10:23am
DET	Pass	10:23am
BAR	Pass	10:23am
BT	Pass	10:23am

Blank Tests

Test	Status	Time
AIR	Pass	10:24am


Printer Tests

Test	Status	Time
PRNT	Pass	10:24am

CRC Tests

Test	Status	Time
COMP	Pass	10:24am
CAL	Pass	10:24am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Macon Instrument Location Macon County Jail
Instrument Serial No. 008618 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008618
Test Date: 12/08/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	1:19pm
AIR BLK	.00	1:20pm
ACCY CHK	.07	1:20pm
AIR BLK	.00	1:21pm
SUB TEST	.00	1:22pm
AIR BLK	.00	1:23pm
SUB TEST	.00	1:24pm
AIR BLK	.00	1:25pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008618 Test Record Number: 2235
Test Date: 12/08/2021 Test Time: 1:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:26pm
FLO	Pass	1:26pm
FC	Pass	1:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:26pm
SRC	Pass	1:26pm
DET	Pass	1:26pm
BAR	Pass	1:26pm
BT	Pass	1:26pm

Blank Tests

Test	Status	Time
AIR	Pass	1:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:27pm

CRC Tests

Test	Status	Time
COMP	Pass	1:27pm
CAL	Pass	1:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Mecon Instrument Location Mecon County Jail

Instrument Serial No. 009789 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 668 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008789
Test Date: 12/08/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	1:21pm
AIR BLK	.00	1:21pm
ACCY CHK	.07	1:22pm
AIR BLK	.00	1:23pm
SUB TEST	.00	1:23pm
AIR BLK	.00	1:25pm
SUB TEST	.00	1:26pm
AIR BLK	.00	1:27pm

Reported AC: .00 g/210L

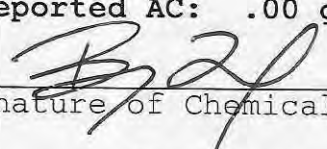

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008789 Test Record Number: 750
Test Date: 12/08/2021 Test Time: 1:28pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:28pm
FLO	Pass	1:28pm
FC	Pass	1:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:28pm
SRC	Pass	1:28pm
DET	Pass	1:28pm
BAR	Pass	1:28pm
BT	Pass	1:28pm

Blank Tests

Test	Status	Time
AIR	Pass	1:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:29pm

CRC Tests

Test	Status	Time
COMP	Pass	1:29pm
CAL	Pass	1:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Macon Instrument Location Macon County Magistrate

Instrument Serial No. 008795 Highlands, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795
Test Date: 12/08/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022


Test	g/210L	Time
DIAG	Pass	12:07pm
AIR BLK	.00	12:08pm
ACCY CHK	.08	12:09pm
AIR BLK	.00	12:10pm
SUB TEST	.00	12:10pm
AIR BLK	.00	12:11pm
SUB TEST	.00	12:13pm
AIR BLK	.00	12:14pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

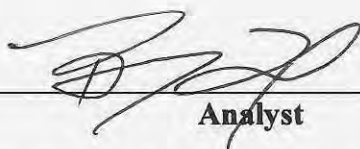

Analyst

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795 Test Record Number: 559
Test Date: 12/08/2021 Test Time: 12:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:14pm
FLO	Pass	12:14pm
FC	Pass	12:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:15pm
SRC	Pass	12:15pm
DET	Pass	12:15pm
BAR	Pass	12:15pm
BT	Pass	12:15pm

Blank Tests

Test	Status	Time
AIR	Pass	12:15pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:15pm

CRC Tests

Test	Status	Time
COMP	Pass	12:15pm
CAL	Pass	12:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Martin Instrument Location Martin Co. S.O.
Instrument Serial No. 008912 305 E. Main St., Williamston
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of December, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ken [Signature] 643
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912

Test Date: 12/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	2:35pm
AIR BLK	.00	2:35pm
ACCY CHK	.08	2:36pm
AIR BLK	.00	2:37pm
SUB TEST	.00	2:38pm
AIR BLK	.00	2:39pm
SUB TEST	.00	2:41pm
AIR BLK	.00	2:42pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912 Test Record Number: 1785
Test Date: 12/03/2021 Test Time: 2:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:43pm
FLO	Pass	2:43pm
FC	Pass	2:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:43pm
SRC	Pass	2:43pm
DET	Pass	2:43pm
BAR	Pass	2:43pm
BT	Pass	2:43pm

Blank Tests

Test	Status	Time
AIR	Pass	2:44pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:44pm

CRC Tests

Test	Status	Time
COMP	Pass	2:44pm
CAL	Pass	2:44pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location CMPD LEC
Instrument Serial No. 0082691 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691
Test Date: 12/15/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	10:53am
AIR BLK	.00	10:53am
ACCY CHK	.08	10:54am
AIR BLK	.00	10:55am
SUB TEST	.00	10:56am
AIR BLK	.00	10:57am
SUB TEST	.00	10:58am
AIR BLK	.00	10:59am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

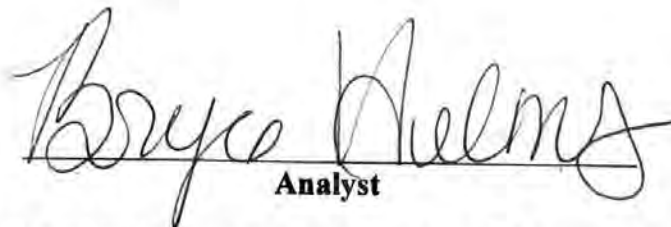
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691 Test Record Number: 8624
Test Date: 12/15/2021 Test Time: 10:59am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00am
FLO	Pass	11:00am
FC	Pass	11:00am

Temperature Tests

Test	Status	Time
FC1	Pass	11:00am
SRC	Pass	11:00am
DET	Pass	11:00am
BAR	Pass	11:00am
BT	Pass	11:00am

Blank Tests

Test	Status	Time
AIR	Pass	11:01am


Printer Tests

Test	Status	Time
PRNT	Pass	11:01am

CRC Tests

Test	Status	Time
COMP	Pass	11:01am
CAL	Pass	11:01am

Preventive Maintenance
Status: *Pass*

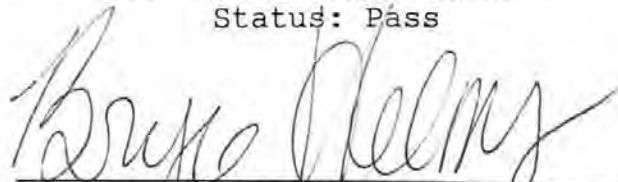

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Cornelius PD
Instrument Serial No. 00810920 Cornelius, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692

Test Date: 12/20/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:07pm
AIR BLK	.00	12:07pm
ACCY CHK	.07	12:08pm
AIR BLK	.00	12:09pm
SUB TEST	.00	12:10pm
AIR BLK	.00	12:11pm
SUB TEST	.00	12:12pm
AIR BLK	.00	12:13pm

Reported AC: .00 g/210L

Bryce Helms

Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692 Test Record Number: 3186
Test Date: 12/20/2021 Test Time: 12:13pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:14pm
FLO	Pass	12:14pm
FC	Pass	12:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:14pm
SRC	Pass	12:14pm
DET	Pass	12:14pm
BAR	Pass	12:14pm
BT	Pass	12:14pm

Blank Tests

Test	Status	Time
AIR	Pass	12:15pm

Printer Tests


Test	Status	Time
PRNT	Pass	12:15pm

CRC Tests

Test	Status	Time
COMP	Pass	12:15pm
CAL	Pass	12:15pm

Preventive Maintenance

Status: *Pass*

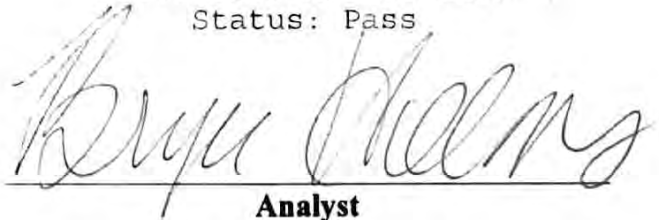

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location BAT MOBILE 6

Instrument Serial No. 008776 CHARLOTTE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. C. Fly
Signature of Certifying Official

676
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 6 590

Serial Number: 008776 Test Record Number: 3715
Test Date: 12/16/2021 Test Time: 10:05pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:05pm
FLO	Pass	10:05pm
FC	Pass	10:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:05pm
SRC	Pass	10:05pm
DET	Pass	10:05pm
BAR	Pass	10:05pm
BT	Pass	10:05pm

Blank Tests

Test	Status	Time
AIR	Pass	10:06pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:06pm

CRC Tests

Test	Status	Time
COMP	Pass	10:06pm
CAL	Pass	10:06pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 6
590

Serial Number: 008776

Test Date: 12/16/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Marshall C

Permit Number: 0027-5012

Effective:

07/16/2021-07/16/2023

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	9:55pm
AIR BLK	.00	9:55pm
ACCY CHK	.07	9:56pm
AIR BLK	.00	9:57pm
SUB TEST	.00	9:57pm
AIR BLK	.00	9:58pm
SUB TEST	.00	10:00pm
AIR BLK	.00	10:01pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Mitchell Instrument Location Spivee Pine Police Dept

Instrument Serial No. 009726 Spivee Pine, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 668 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MITCHELL COUNTY SPRUCE PINE PD 600

Serial Number: 008726

Test Date: 12/20/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	10:25am
AIR BLK	.00	10:25am
ACCY CHK	.08	10:26am
AIR BLK	.00	10:27am
SUB TEST	.00	10:27am
AIR BLK	.00	10:28am
SUB TEST	.00	10:30am
AIR BLK	.00	10:31am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MITCHELL COUNTY SPRUCE PINE PD 600

Serial Number: 008726 Test Record Number: 1190
Test Date: 12/20/2021 Test Time: 10:32am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:32am
FLO	Pass	10:32am
FC	Pass	10:32am

Temperature Tests

Test	Status	Time
FC1	Pass	10:33am
SRC	Pass	10:33am
DET	Pass	10:33am
BAR	Pass	10:33am
BT	Pass	10:33am

Blank Tests

Test	Status	Time
AIR	Pass	10:33am

Printer Tests

Test	Status	Time
PRNT	Pass	10:33am

CRC Tests

Test	Status	Time
COMP	Pass	10:33am
CAL	Pass	10:33am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County New Hanover Instrument Location New Hanover County
Instrument Serial No. 008626 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008626
Test Date: 12/14/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	4:03pm
AIR BLK	.00	4:04pm
ACCY CHK	.08	4:04pm
AIR BLK	.00	4:05pm
SUB TEST	.00	4:06pm
AIR BLK	.00	4:07pm
SUB TEST	.00	4:08pm
AIR BLK	.00	4:09pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008626 Test Record Number: 8075
Test Date: 12/14/2021 Test Time: 4:10pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:10pm
FLO	Pass	4:10pm
FC	Pass	4:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:10pm
SRC	Pass	4:10pm
DET	Pass	4:10pm
BAR	Pass	4:10pm
BT	Pass	4:10pm

Blank Tests

Test	Status	Time
AIR	Pass	4:11pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:11pm

CRC Tests

Test	Status	Time
COMP	Pass	4:11pm
CAL	Pass	4:11pm

Preventive Maintenance
Status: Pass

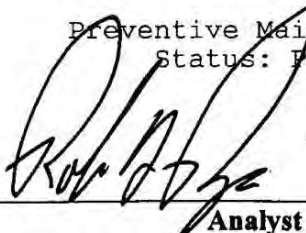

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County New Hanover Instrument Location New Hanover County
Instrument Serial No. 008628 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008628
Test Date: 12/11/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	9:18pm
AIR BLK	.00	9:18pm
ACCY CHK	.08	9:19pm
AIR BLK	.00	9:20pm
SUB TEST	.00	9:20pm
AIR BLK	.00	9:21pm
SUB TEST	.00	9:23pm
AIR BLK	.00	9:24pm

Reported AC  .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008628 Test Record Number: 5738
Test Date: 12/11/2021 Test Time: 9:24pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:25pm
FLO	Pass	9:25pm
FC	Pass	9:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:25pm
SRC	Pass	9:25pm
DET	Pass	9:25pm
BAR	Pass	9:25pm
BT	Pass	9:25pm

Blank Tests

Test	Status	Time
AIR	Pass	9:26pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:26pm

CRC Tests

Test	Status	Time
COMP	Pass	9:26pm
CAL	Pass	9:26pm

Preventive Maintenance
Status: *Pass*



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County New Hanover Instrument Location Wrightsville Beach
Instrument Serial No. 008667 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of December, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD
640

Serial Number: 008667
Test Date: 12/21/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	4:05pm
AIR BLK	.00	4:06pm
ACCY CHK	.07	4:06pm
AIR BLK	.00	4:07pm
SUB TEST	.00	4:08pm
AIR BLK	.00	4:09pm
SUB TEST	.00	4:11pm
AIR BLK	.00	4:11pm

Reported AC: .00 g/210L

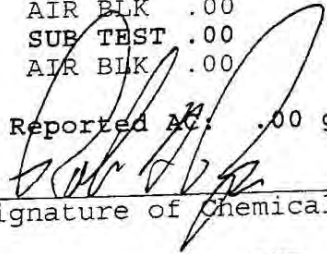

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD 640

Serial Number: 008667. Test Record Number: 2198
Test Date: 12/21/2021 Test Time: 4:12pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	4:13pm
FLO	Pass	4:13pm
FC	Pass	4:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:13pm
SRC	Pass	4:13pm
DET	Pass	4:13pm
BAR	Pass	4:13pm
BT	Pass	4:13pm

Blank Tests

Test	Status	Time
AIR	Pass	4:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:14pm

CRC Tests

Test	Status	Time
COMP	Pass	4:14pm
CAL	Pass	4:14pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County New Hanover Instrument Location Carolina Beach
Instrument Serial No. 008901 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY CAROLINA BEACH PD
640

Serial Number: 008901
Test Date: 12/21/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	2:59pm
AIR BLK	.00	3:00pm
ACCY CHK	.08	3:01pm
AIR BLK	.00	3:02pm
SUB TEST	.00	3:02pm
AIR BLK	.00	3:03pm
SUB TEST	.00	3:05pm
AIR BLK	.00	3:06pm

Reported AC# .00 g/210L

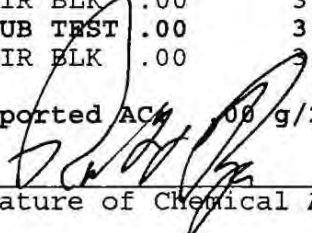

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY CAROLINA BEACH PD 640

Serial Number: 008901 Test Record Number: 1490
Test Date: 12/21/2021 Test Time: 3:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:07pm
FLO	Pass	3:07pm
FC	Pass	3:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:07pm
SRC	Pass	3:07pm
DET	Pass	3:07pm
BAR	Pass	3:07pm
BT	Pass	3:07pm

Blank Tests

Test	Status	Time
AIR	Pass	3:08pm

Printer Tests


Test	Status	Time
PRNT	Pass	3:08pm

CRC Tests

Test	Status	Time
COMP	Pass	3:08pm
CAL	Pass	3:08pm

Preventive Maintenance

Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County New Hanover Instrument Location BAT Mobile Unit 6
Instrument Serial No. 008686 Wilmington

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY BAT MOBILE UNIT 6
640

Serial Number: 008686
Test Date: 12/31/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	11:03pm
AIR BLK	.00	11:04pm
ACCY CHK	.08	11:04pm
AIR BLK	.00	11:05pm
SUB TEST	.00	11:06pm
AIR BLK	.00	11:07pm
SUB TEST	.00	11:08pm
AIR BLK	.00	11:09pm

Reported AC: .00 g/210L

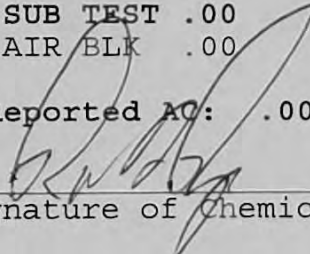

Signature of Chemical Analyst

Court CVR

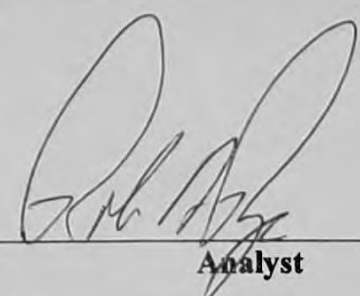

Analyst

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY BAT MOBILE UNIT 6 640

Serial Number: 008686 Test Record Number: 6828
Test Date: 12/31/2021 Test Time: 11:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:13pm
FLO	Pass	11:13pm
FC	Pass	11:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:13pm
SRC	Pass	11:13pm
DET	Pass	11:13pm
BAR	Pass	11:13pm
BT	Pass	11:13pm

Blank Tests

Test	Status	Time
AIR	Pass	11:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:13pm

CRC Tests

Test	Status	Time
COMP	Pass	11:14pm
CAL	Pass	11:14pm

Preventive Maintenance
Status: Pass

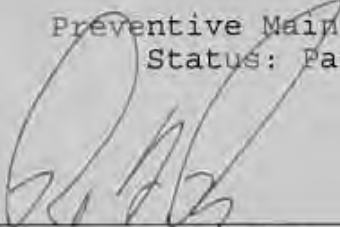

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County New Hanover Instrument Location BAT Mobile Unit 6
Instrument Serial No. 008776 Wilmington

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus 2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY BAT MOBILE UNIT 6
640

Serial Number: 008776
Test Date: 12/31/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	11:07pm
AIR BLK	.00	11:08pm
ACCY CHK	.07	11:08pm
AIR BLK	.00	11:09pm
SUB TEST	.00	11:10pm
AIR BLK	.00	11:11pm
SUB TEST	.00	11:12pm
AIR BLK	.00	11:13pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY BAT MOBILE UNIT 6 640

Serial Number: 008776 Test Record Number: 3735
Test Date: 12/31/2021 Test Time: 11:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:17pm
FLO	Pass	11:17pm
FC	Pass	11:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:17pm
SRC	Pass	11:17pm
DET	Pass	11:17pm
BAR	Pass	11:17pm
BT	Pass	11:17pm

Blank Tests

Test	Status	Time
AIR	Pass	11:17pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:17pm

CRC Tests

Test	Status	Time
COMP	Pass	11:18pm
CAL	Pass	11:18pm

Preventive Maintenance
Status: Pass

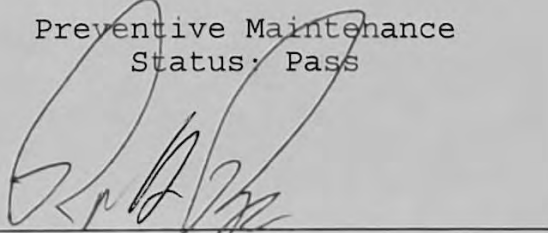

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008698 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: 008698

Test Date: 12/31/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	8:29pm
AIR BLK	.00	8:30pm
ACCY CHK	.08	8:31pm
AIR BLK	.00	8:32pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:35pm
AIR BLK	.00	8:35pm

Reported AC: .00 g/210L

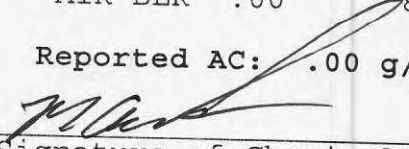

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE 12 660

Serial Number: 008698 Test Record Number: 1750
Test Date: 12/31/2021 Test Time: 8:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:37pm
FLO	Pass	8:37pm
FC	Pass	8:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:37pm
SRC	Pass	8:37pm
DET	Pass	8:37pm
BAR	Pass	8:37pm
BT	Pass	8:37pm

Blank Tests

Test	Status	Time
AIR	Pass	8:38pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:38pm

CRC Tests

Test	Status	Time
COMP	Pass	8:38pm
CAL	Pass	8:38pm

Preventive Maintenance
Status: *Pass*

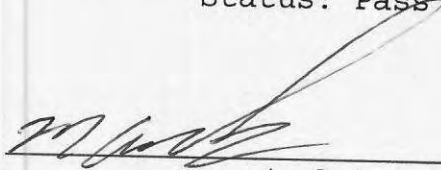

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County onslow Instrument Location BAT mobile unit 72

Instrument Serial No. 008288 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008788
Test Date: 12/31/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	8:23pm
AIR BLK	.00	8:24pm
ACCY CHK	.08	8:24pm
AIR BLK	.00	8:25pm
SUB TEST	.00	8:26pm
AIR BLK	.00	8:27pm
SUB TEST	.00	8:29pm
AIR BLK	.00	8:29pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008788 Test Record Number: 1718
Test Date: 12/31/2021 Test Time: 8:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:32pm
FLO	Pass	8:32pm
FC	Pass	8:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:32pm
SRC	Pass	8:32pm
DET	Pass	8:32pm
BAR	Pass	8:32pm
BT	Pass	8:32pm

Blank Tests

Test	Status	Time
AIR	Pass	8:33pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:33pm

CRC Tests

Test	Status	Time
COMP	Pass	8:33pm
CAL	Pass	8:33pm

Preventive Maintenance
Status: Pass

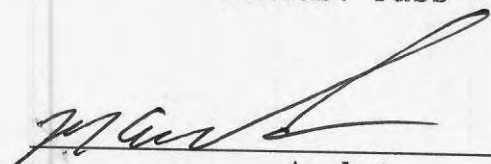

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLOW Instrument Location MCA5 NEW RIVER

Instrument Serial No. 008919 PMD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of DECEMBER, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alvin B. [Signature]
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919
Test Date: 12/14/2021

Citation Number: M0000000-0

Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG131901
Exp Date: 11/15/2023


Test	g/210L	Time
DIAG	Pass	11:52am
AIR BLK	.00	11:53am
ACCY CHK	.08	11:53am
AIR BLK	.00	11:54am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am
SUB TEST	.00	11:57am
AIR BLK	.00	11:58am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY MCAS NEW RIVER 660

Serial Number: 008919 Test Record Number: 774
Test Date: 12/14/2021 Test Time: 11:59am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:59am
FLO	Pass	11:59am
FC	Pass	11:59am

Temperature Tests

Test	Status	Time
FC1	Pass	11:59am
SRC	Pass	11:59am
DET	Pass	11:59am
BAR	Pass	11:59am
BT	Pass	11:59am

Blank Tests

Test	Status	Time
AIR	Pass	12:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:00pm

CRC Tests

Test	Status	Time
COMP	Pass	12:00pm
CAL	Pass	12:00pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLOW Instrument Location CAMP LEJEUNE
Instrument Serial No. 008920 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John R. Barnes

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920
Test Date: 12/14/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG131901
Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	1:44pm
AIR BLK	.00	1:45pm
ACCY CHK	.08	1:45pm
AIR BLK	.00	1:46pm
SUB TEST	.00	1:47pm
AIR BLK	.00	1:48pm
SUB TEST	.00	1:49pm
AIR BLK	.00	1:50pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920 Test Record Number: 1916
Test Date: 12/14/2021 Test Time: 1:50pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:51pm
FLO	Pass	1:51pm
FC	Pass	1:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:51pm
SRC	Pass	1:51pm
DET	Pass	1:51pm
BAR	Pass	1:51pm
BT	Pass	1:51pm

Blank Tests

Test	Status	Time
AIR	Pass	1:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:52pm

CRC Tests

Test	Status	Time
COMP	Pass	1:52pm
CAL	Pass	1:52pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSLow Instrument Location JACKSONVILLE

Instrument Serial No. 008930 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY JACKSONVILLE PD 660

Serial Number: 008930
Test Date: 12/14/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	3:04pm
AIR BLK	.00	3:04pm
ACCY CHK	.08	3:05pm
AIR BLK	.00	3:06pm
SUB TEST	.00	3:07pm
AIR BLK	.00	3:08pm
SUB TEST	.00	3:09pm
AIR BLK	.00	3:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY JACKSONVILLE PD 660

Serial Number: 008930 Test Record Number: 2139
Test Date: 12/14/2021 Test Time: 3:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:11pm
FLO	Pass	3:11pm
FC	Pass	3:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:12pm
SRC	Pass	3:12pm
DET	Pass	3:12pm
BAR	Pass	3:12pm
BT	Pass	3:12pm

Blank Tests

Test	Status	Time
AIR	Pass	3:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:12pm

CRC Tests

Test	Status	Time
COMP	Pass	3:12pm
CAL	Pass	3:12pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONslow Instrument Location ONslow COUNTY

Instrument Serial No. 008931 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 03 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ON SLOW COUNTY DETENTION CENTER 660

Serial Number: 008931
Test Date: 12/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	1:18pm
AIR BLK	.00	1:19pm
ACCY CHK	.08	1:20pm
AIR BLK	.00	1:21pm
SUB TEST	.00	1:22pm
AIR BLK	.00	1:22pm
SUB TEST	.00	1:24pm
AIR BLK	.00	1:25pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931 Test Record Number: 3745
Test Date: 12/03/2021 Test Time: 1:28pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:28pm
FLO	Pass	1:28pm
FC	Pass	1:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:28pm
SRC	Pass	1:28pm
DET	Pass	1:28pm
BAR	Pass	1:28pm
BT	Pass	1:28pm

Blank Tests

Test	Status	Time
AIR	Pass	1:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:29pm

CRC Tests

Test	Status	Time
COMP	Pass	1:29pm
CAL	Pass	1:29pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSLow Instrument Location ONSLow COUNTY

Instrument Serial No. 008932 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 03 day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alvin B...

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008932
Test Date: 12/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	1:12pm
AIR BLK	.00	1:12pm
ACCY CHK	.08	1:13pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:15pm
AIR BLK	.00	1:16pm
SUB TEST	.00	1:17pm
AIR BLK	.00	1:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008932 Test Record Number: 6516
Test Date: 12/03/2021 Test Time: 1:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:19pm
FLO	Pass	1:19pm
FC	Pass	1:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:19pm
SRC	Pass	1:19pm
DET	Pass	1:19pm
BAR	Pass	1:19pm
BT	Pass	1:19pm

Blank Tests

Test	Status	Time
AIR	Pass	1:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:20pm

CRC Tests

Test	Status	Time
COMP	Pass	1:20pm
CAL	Pass	1:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pender Instrument Location Pender County
Instrument Serial No. 008935 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY DETENTION CENTER 700

Serial Number: 008935
Test Date: 12/13/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107501
Exp Date: 03/16/2023


Test	g/210L	Time
DIAG	Pass	3:01pm
AIR BLK	.00	3:02pm
ACCY CHK	.07	3:02pm
AIR BLK	.00	3:03pm
SUB TEST	.00	3:04pm
AIR BLK	.00	3:05pm
SUB TEST	.00	3:06pm
AIR BLK	.00	3:07pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY DETENTION CENTER 700

Serial Number: 008935 Test Record Number: 2955
Test Date: 12/13/2021 Test Time: 3:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:08pm
FLO	Pass	3:08pm
FC	Pass	3:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:08pm
SRC	Pass	3:08pm
DET	Pass	3:08pm
BAR	Pass	3:08pm
BT	Pass	3:08pm

Blank Tests

Test	Status	Time
AIR	Pass	3:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:09pm

CRC Tests

Test	Status	Time
COMP	Pass	3:09pm
CAL	Pass	3:09pm

Preventive Maintenance
Status: *Pass*



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pender Instrument Location Pender County
Instrument Serial No. 008948 Government Annex

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY GOVERNMENT ANNEX 700

Serial Number: 008948
Test Date: 12/13/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	1:22pm
AIR BLK	.00	1:23pm
ACCY CHK	.07	1:24pm
AIR BLK	.00	1:25pm
SUB TEST	.00	1:25pm
AIR BLK	.00	1:26pm
SUB TEST	.00	1:28pm
AIR BLK	.00	1:29pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY GOVERNMENT ANNEX 700

Serial Number: 008948 Test Record Number: 1228
Test Date: 12/13/2021 Test Time: 1:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:31pm
FLO	Pass	1:31pm
FC	Pass	1:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:31pm
SRC	Pass	1:31pm
DET	Pass	1:31pm
BAR	Pass	1:31pm
BT	Pass	1:31pm

Blank Tests

Test	Status	Time
AIR	Pass	1:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:32pm

CRC Tests

Test	Status	Time
COMP	Pass	1:32pm
CAL	Pass	1:32pm

Preventive Maintenance

Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County P.H. Instrument Location P.H. Co. Detention Center

Instrument Serial No. D091646 174 New Hope Rd. Grassville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646

Test Date: 12/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	10:05am
AIR BLK	.00	10:06am
ACCY CHK	.08	10:07am
AIR BLK	.00	10:08am
SUB TEST	.00	10:09am
AIR BLK	.00	10:09am
SUB TEST	.00	10:11am
AIR BLK	.00	10:12am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646 Test Record Number: 4339
Test Date: 12/17/2021 Test Time: 10:12am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:13am
FLO	Pass	10:13am
FC	Pass	10:13am

Temperature Tests

Test	Status	Time
FC1	Pass	10:13am
SRC	Pass	10:13am
DET	Pass	10:13am
BAR	Pass	10:13am
BT	Pass	10:13am

Blank Tests

Test	Status	Time
AIR	Pass	10:14am

Printer Tests

Test	Status	Time
PRNT	Pass	10:14am

CRC Tests

Test	Status	Time
COMP	Pass	10:14am
CAL	Pass	10:14am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County P.H. Instrument Location P.H. Correction Center

Instrument Serial No. W8662 124 New Hope Rd, Greenville, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662
Test Date: 12/17/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	10:34am
AIR BLK	.00	10:34am
ACCY CHK	.07	10:35am
AIR BLK	.00	10:36am
SUB TEST	.00	10:37am
AIR BLK	.00	10:38am
SUB TEST	.00	10:39am
AIR BLK	.00	10:40am

Reported AC: ~~.00~~ g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662 Test Record Number: 1247
Test Date: 12/17/2021 Test Time: 10:41am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:41am
FLO	Pass	10:42am
FC	Pass	10:42am

Temperature Tests

Test	Status	Time
FC1	Pass	10:42am
SRC	Pass	10:42am
DET	Pass	10:42am
BAR	Pass	10:42am
BT	Pass	10:42am

Blank Tests

Test	Status	Time
AIR	Pass	10:42am


Printer Tests

Test	Status	Time
PRNT	Pass	10:42am

CRC Tests

Test	Status	Time
COMP	Pass	10:43am
CAL	Pass	10:43am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County P.H. Instrument Location P.H. Co. Detention Center
Instrument Serial No. 1218668 124 New Hope Rd, Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668
Test Date: 12/17/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Guard, Kelly G
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107501
Exp Date: 03/16/2023


Test	g/210L	Time
DIAG	Pass	9:31am
AIR BLK	.00	9:32am
ACCY CHK	.07	9:32am
AIR BLK	.00	9:34am
SUB TEST	.00	9:35am
AIR BLK	.00	9:35am
SUB TEST	.00	9:37am
AIR BLK	.00	9:38am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668 Test Record Number: 4152
Test Date: 12/17/2021 Test Time: 9:39am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:39am
FLO	Pass	9:39am
FC	Pass	9:39am

Temperature Tests

Test	Status	Time
FC1	Pass	9:39am
SRC	Pass	9:39am
DET	Pass	9:39am
BAR	Pass	9:39am
BT	Pass	9:39am

Blank Tests

Test	Status	Time
AIR	Pass	9:40am

Printer Tests

Test	Status	Time
PRNT	Pass	9:40am

CRC Tests

Test	Status	Time
COMP	Pass	9:40am
CAL	Pass	9:40am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Richmond Instrument Location Richmond County

Instrument Serial No. 008701 Magistrates Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RICHMOND COUNTY MAGISTRATE'S OFFICE
760

Serial Number: 008701
Test Date: 12/13/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
03/10/2021-03/10/2023

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG132001
Exp Date: 11/16/2023


Test	g/210L	Time
DIAG	Pass	3:10pm
AIR BLK	.00	3:11pm
ACCY CHK	.08	3:11pm
AIR BLK	.00	3:12pm
SUB TEST	.00	3:13pm
AIR BLK	.00	3:14pm
SUB TEST	.00	3:15pm
AIR BLK	.00	3:16pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

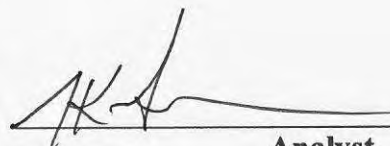

Analyst

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY MAGISTRATE'S OFFICE 760

Serial Number: 008701 Test Record Number: 1284
Test Date: 12/13/2021 Test Time: 3:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:17pm
FLO	Pass	3:17pm
FC	Pass	3:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:17pm
SRC	Pass	3:17pm
DET	Pass	3:17pm
BAR	Pass	3:17pm
BT	Pass	3:17pm

Blank Tests

Test	Status	Time
AIR	Pass	3:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:18pm

CRC Tests

Test	Status	Time
COMP	Pass	3:18pm
CAL	Pass	3:18pm

Preventive Maintenance
Status: Pass

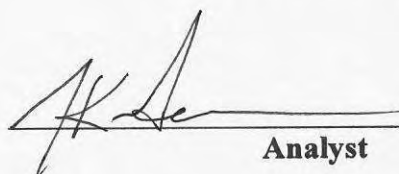

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Richmond Instrument Location Richmond County
Instrument Serial No. 008840 Magistrates Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



AK Aa
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RICHMOND COUNTY MAGISTRATE'S OFFICE
760

Serial Number: 008840
Test Date: 12/13/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
03/10/2021-03/10/2023

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG132001
Exp Date: 11/16/2023


Test	g/210L	Time
DIAG	Pass	3:07pm
AIR BLK	.00	3:08pm
ACCY CHK	.07	3:08pm
AIR BLK	.00	3:09pm
SUB TEST	.00	3:10pm
AIR BLK	.00	3:11pm
SUB TEST	.00	3:12pm
AIR BLK	.00	3:13pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

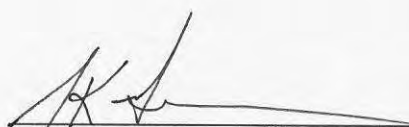

Analyst

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY MAGISTRATE'S OFFICE 760

Serial Number: 008840 Test Record Number: 2664
Test Date: 12/13/2021 Test Time: 3:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:14pm
FLO	Pass	3:14pm
FC	Pass	3:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:14pm
SRC	Pass	3:14pm
DET	Pass	3:14pm
BAR	Pass	3:14pm
BT	Pass	3:14pm

Blank Tests

Test	Status	Time
AIR	Pass	3:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:15pm

CRC Tests

Test	Status	Time
COMP	Pass	3:15pm
CAL	Pass	3:15pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT mobile Unit #5


Instrument Serial No. 008525 Lumberton Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

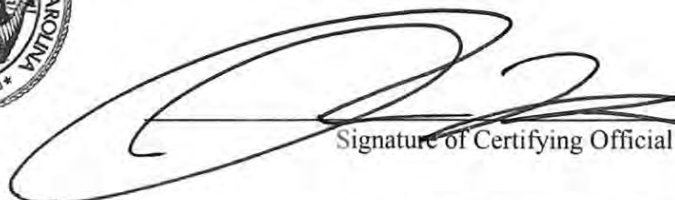


Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008575
Test Date: 12/31/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	9:30pm
AIR BLK	.00	9:31pm
ACCY CHK	.08	9:32pm
AIR BLK	.00	9:33pm
SUB TEST	.00	9:33pm
AIR BLK	.00	9:34pm
SUB TEST	.00	9:36pm
AIR BLK	.00	9:37pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

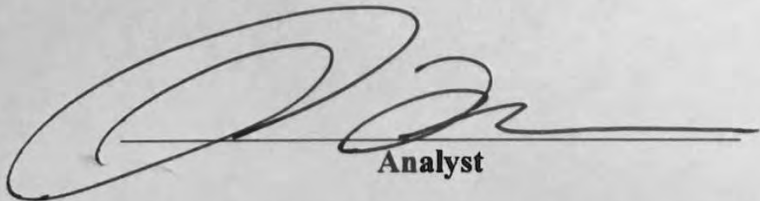
Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008575 Test Record Number: 1291
Test Date: 12/31/2021 Test Time: 9:38pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:38pm
FLO	Pass	9:38pm
FC	Pass	9:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:38pm
SRC	Pass	9:38pm
DET	Pass	9:38pm
BAR	Pass	9:38pm
BT	Pass	9:38pm

Blank Tests

Test	Status	Time
AIR	Pass	9:39pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:39pm

CRC Tests

Test	Status	Time
COMP	Pass	9:39pm
CAL	Pass	9:39pm

Preventive Maintenance
Status: Pass

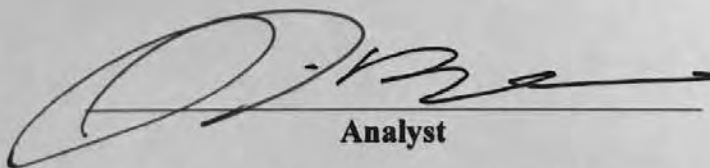

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location Lumberton Police
Instrument Serial No. 008629 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY LUMBERTON PD 770

Serial Number: 008629

Test Date: 12/10/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

03/10/2021-03/10/2023

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034901

Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	9:54am
AIR BLK	.00	9:54am
ACCY CHK	.07	9:55am
AIR BLK	.00	9:56am
SUB TEST	.00	9:57am
AIR BLK	.00	9:58am
SUB TEST	.00	9:59am
AIR BLK	.00	10:00am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY LUMBERTON PD 770

Serial Number: 008629 Test Record Number: 1078
Test Date: 12/10/2021 Test Time: 10:01am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:01am
FLO	Pass	10:01am
FC	Pass	10:01am

Temperature Tests

Test	Status	Time
FC1	Pass	10:01am
SRC	Pass	10:01am
DET	Pass	10:01am
BAR	Pass	10:01am
BT	Pass	10:01am

Blank Tests

Test	Status	Time
AIR	Pass	10:02am


Printer Tests

Test	Status	Time
PRNT	Pass	10:02am

CRC Tests

Test	Status	Time
COMP	Pass	10:02am
CAL	Pass	10:02am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit # 5
Instrument Serial No. 008826 Robeson County Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 664
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826
Test Date: 12/08/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002


Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	5:04pm
AIR BLK	.00	5:05pm
ACCY CHK	.08	5:06pm
AIR BLK	.00	5:07pm
SUB TEST	.00	5:08pm
AIR BLK	.00	5:09pm
SUB TEST	.00	5:11pm
AIR BLK	.00	5:12pm

Reported AC: .00 g/210L

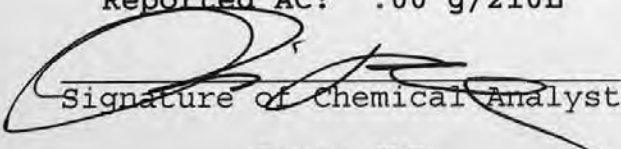
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826 Test Record Number: 8393
Test Date: 12/08/2021 Test Time: 5:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:13pm
FLO	Pass	5:13pm
FC	Pass	5:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:13pm
SRC	Pass	5:13pm
DET	Pass	5:13pm
BAR	Pass	5:13pm
BT	Pass	5:13pm

Blank Tests

Test	Status	Time
AIR	Pass	5:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:14pm

CRC Tests

Test	Status	Time
COMP	Pass	5:14pm
CAL	Pass	5:14pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROWAN Instrument Location CHINA GROVE

Instrument Serial No. 008862 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7TH day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862
Test Date: 12/07/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107502

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	9:57am
AIR BLK	.00	9:58am
ACCY CHK	.07	9:59am
AIR BLK	.00	10:00am
SUB TEST	.00	10:00am
AIR BLK	.00	10:02am
SUB TEST	.00	10:03am
AIR BLK	.00	10:04am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862 Test Record Number: 1000
Test Date: 12/07/2021 Test Time: 10:04am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:05am
FLO	Pass	10:05am
FC	Pass	10:05am

Temperature Tests

Test	Status	Time
FC1	Pass	10:05am
SRC	Pass	10:05am
DET	Pass	10:05am
BAR	Pass	10:05am
BT	Pass	10:05am

Blank Tests

Test	Status	Time
AIR	Pass	10:06am


Printer Tests

Test	Status	Time
PRNT	Pass	10:06am

CRC Tests

Test	Status	Time
COMP	Pass	10:06am
CAL	Pass	10:06am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Sampson Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008616 Clinton Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are;

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 608 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008616
Test Date: 12/13/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Todd, Shane C
Permit Number: 0035-4789
Effective:
10/06/2020-10/06/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG132002
Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	5:15pm
AIR BLK	.00	5:16pm
ACCY CHK	.08	5:16pm
AIR BLK	.00	5:17pm
SUB TEST	.00	5:18pm
AIR BLK	.00	5:19pm
SUB TEST	.00	5:20pm
AIR BLK	.00	5:21pm

Reported AC: .00 g/210L

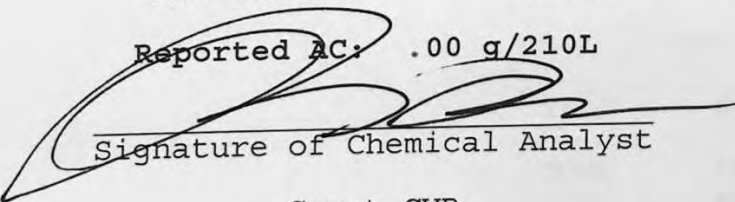
Signature of Chemical Analyst

Court CVR

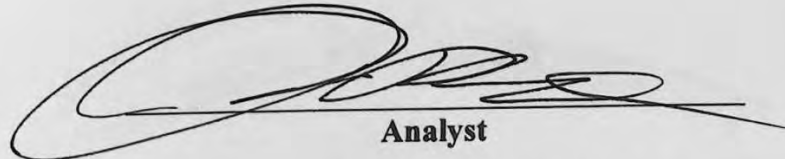
Analyst

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008616 Test Record Number: 2669
Test Date: 12/13/2021 Test Time: 5:23pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:24pm
FLO	Pass	5:24pm
FC	Pass	5:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:24pm
SRC	Pass	5:24pm
DET	Pass	5:24pm
BAR	Pass	5:24pm
BT	Pass	5:24pm

Blank Tests

Test	Status	Time
AIR	Pass	5:24pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:25pm

CRC Tests

Test	Status	Time
COMP	Pass	5:25pm
CAL	Pass	5:25pm

Preventive Maintenance
Status: Pass

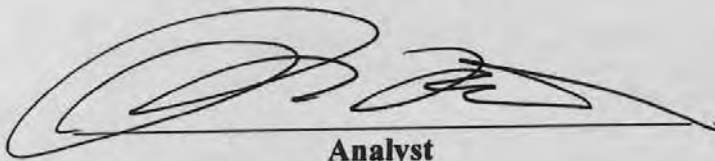

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Sampson Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008826 Clinton Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008826
Test Date: 12/13/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG132002


Exp Date: 11/16/2023

Test	g/210L	Time
DIAG	Pass	5:07pm
AIR BLK	.00	5:08pm
ACCY CHK	.08	5:08pm
AIR BLK	.00	5:09pm
SUB TEST	.00	5:10pm
AIR BLK	.00	5:11pm
SUB TEST	.00	5:12pm
AIR BLK	.00	5:13pm

Reported AC: .00 g/210L

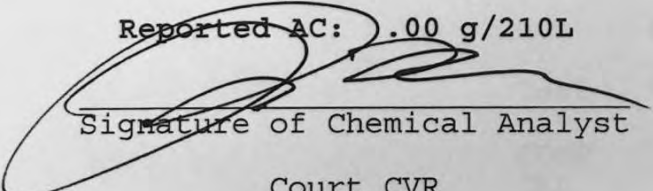
Signature of Chemical Analyst

Court CVR

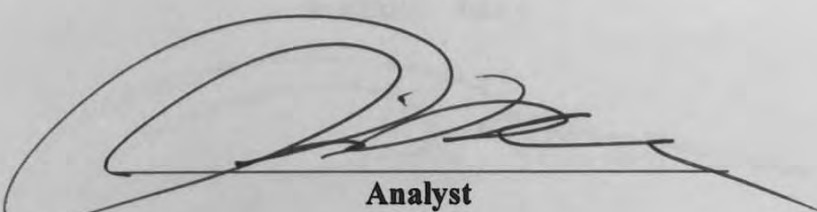
Analyst

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008826 Test Record Number: 8397
Test Date: 12/13/2021 Test Time: 5:15pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:15pm
FLO	Pass	5:15pm
FC	Pass	5:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:15pm
SRC	Pass	5:15pm
DET	Pass	5:15pm
BAR	Pass	5:15pm
BT	Pass	5:15pm

Blank Tests

Test	Status	Time
AIR	Pass	5:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:16pm

CRC Tests

Test	Status	Time
COMP	Pass	5:16pm
CAL	Pass	5:16pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Sampson Instrument Location Sampson County
Instrument Serial No. 008825 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of December, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825
Test Date: 12/07/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	11:47am
AIR BLK	.00	11:48am
ACCY CHK	.07	11:48am
AIR BLK	.00	11:49am
SUB TEST	.00	11:50am
AIR BLK	.00	11:51am
SUB TEST	.00	11:52am
AIR BLK	.00	11:53am

Reported AC: .00 g/210L

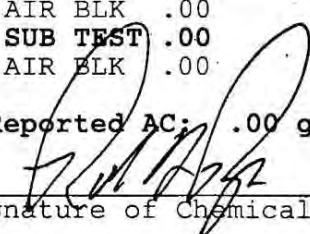

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825 Test Record Number: 3330
Test Date: 12/07/2021 Test Time: 11:54am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:54am
FLO	Pass	11:54am
FC	Pass	11:54am

Temperature Tests

Test	Status	Time
FC1	Pass	11:55am
SRC	Pass	11:55am
DET	Pass	11:55am
BAR	Pass	11:55am
BT	Pass	11:55am

Blank Tests

Test	Status	Time
AIR	Pass	11:55am

Printer Tests

Test	Status	Time
PRNT	Pass	11:55am

CRC Tests

Test	Status	Time
COMP	Pass	11:55am
CAL	Pass	11:55am

Preventive Maintenance
Status: *Pass*



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Sampson Instrument Location Sampson County
Instrument Serial No. 008877 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877
Test Date: 12/07/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118804
Exp Date: 07/07/2023


Test	g/210L	Time
DIAG	Pass	11:45am
AIR BLK	.00	11:45am
ACCY CHK	.08	11:46am
AIR BLK	.00	11:47am
SUB TEST	.00	11:48am
AIR BLK	.00	11:49am
SUB TEST	.00	11:50am
AIR BLK	.00	11:51am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

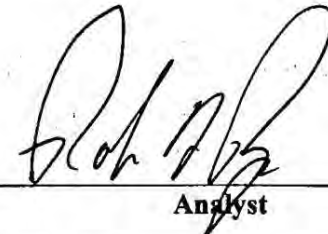

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877 Test Record Number: 3548
Test Date: 12/07/2021 Test Time: 11:52am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:52am
FLO	Pass	11:52am
FC	Pass	11:52am

Temperature Tests

Test	Status	Time
FC1	Pass	11:52am
SRC	Pass	11:52am
DET	Pass	11:52am
BAR	Pass	11:52am
BT	Pass	11:52am

Blank Tests

Test	Status	Time
AIR	Pass	11:53am


Printer Tests

Test	Status	Time
PRNT	Pass	11:53am

CRC Tests

Test	Status	Time
COMP	Pass	11:53am
CAL	Pass	11:53am

Preventive Maintenance
Status: Pass

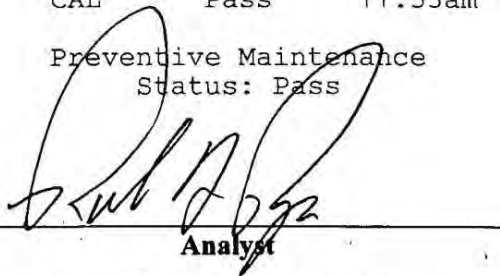

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County STOKES Instrument Location STOKES COUNTY JAIL

Instrument Serial No. 008596 DANBURY, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10TH day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596
Test Date: 12/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	2:23pm
AIR BLK	.00	2:24pm
ACCY CHK	.07	2:24pm
AIR BLK	.00	2:25pm
SUB TEST	.00	2:26pm
AIR BLK	.00	2:27pm
SUB TEST	.00	2:28pm
AIR BLK	.00	2:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596 Test Record Number: 1235
Test Date: 12/10/2021 Test Time: 2:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:31pm
FLO	Pass	2:31pm
FC	Pass	2:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:31pm
SRC	Pass	2:31pm
DET	Pass	2:31pm
BAR	Pass	2:31pm
BT	Pass	2:31pm

Blank Tests

Test	Status	Time
AIR	Pass	2:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:32pm

CRC Tests

Test	Status	Time
COMP	Pass	2:32pm
CAL	Pass	2:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County STOKES Instrument Location KING POLICE

Instrument Serial No. 008718 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10TH day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY KING P D 840

Serial Number: 008718
Test Date: 12/10/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	3:29pm
AIR BLK	.00	3:30pm
ACCY CHK	.07	3:30pm
AIR BLK	.00	3:31pm
SUB TEST	.00	3:32pm
AIR BLK	.00	3:33pm
SUB TEST	.00	3:35pm
AIR BLK	.00	3:36pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY KING P D 840

Serial Number: 008718 Test Record Number: 2165
Test Date: 12/10/2021 Test Time: 3:37pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:37pm
FLO	Pass	3:37pm
FC	Pass	3:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:38pm
SRC	Pass	3:38pm
DET	Pass	3:38pm
BAR	Pass	3:38pm
BT	Pass	3:38pm

Blank Tests

Test	Status	Time
AIR	Pass	3:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:38pm

CRC Tests

Test	Status	Time
COMP	Pass	3:38pm
CAL	Pass	3:38pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County SURRY Instrument Location SURRY COUNTY JAIL
Instrument Serial No. 008934 DOBSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17TH day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY SURRY CO JAIL 850

Serial Number: 008934
Test Date: 12/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: *Oligmueller Jr., Leo A*

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: *Breath Test*

Lot Number: AG131901

Exp Date: 11/15/2023

Test	g/210L	Time
DIAG	Pass	10:57am
AIR BLK	.00	10:58am
ACCY CHK	.08	10:59am
AIR BLK	.00	10:59am
SUB TEST	.00	11:00am
AIR BLK	.00	11:01am
SUB TEST	.00	11:02am
AIR BLK	.00	11:03am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY SURRY CO JAIL 850

Serial Number: 008934 Test Record Number: 2269
Test Date: 12/17/2021 Test Time: 11:11am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:12am
FLO	Pass	11:12am
FC	Pass	11:12am

Temperature Tests

Test	Status	Time
FC1	Pass	11:12am
SRC	Pass	11:12am
DET	Pass	11:12am
BAR	Pass	11:12am
BT	Pass	11:12am

Blank Tests

Test	Status	Time
AIR	Pass	11:13am

Printer Tests

Test	Status	Time
PRNT	Pass	11:13am

CRC Tests

Test	Status	Time
COMP	Pass	11:13am
CAL	Pass	11:13am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County SURRY Instrument Location PILOT MOUNTAIN

Instrument Serial No. 008938 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17TH day of DECEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938

Test Date: 12/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	2:59pm
AIR BLK	.00	3:00pm
ACCY CHK	.08	3:01pm
AIR BLK	.00	3:02pm
SUB TEST	.00	3:03pm
AIR BLK	.00	3:04pm
SUB TEST	.00	3:07pm
AIR BLK	.00	3:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938 Test Record Number: 749
Test Date: 12/17/2021 Test Time: 3:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:09pm
FLO	Pass	3:09pm
FC	Pass	3:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:09pm
SRC	Pass	3:09pm
DET	Pass	3:09pm
BAR	Pass	3:09pm
BT	Pass	3:09pm

Blank Tests

Test	Status	Time
AIR	Pass	3:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:10pm

CRC Tests

Test	Status	Time
COMP	Pass	3:10pm
CAL	Pass	3:10pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Stallings PD
Instrument Serial No. 008694 Stallings, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Williams
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY STALLINGS PD 890

Serial Number: 008694

Test Date: 12/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001


Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	12:17pm
AIR BLK	.00	12:18pm
ACCY CHK	.07	12:18pm
AIR BLK	.00	12:20pm
SUB TEST	.00	12:20pm
AIR BLK	.00	12:21pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

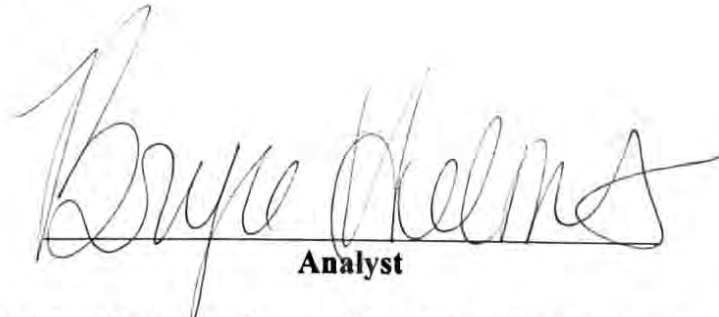
Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY STALLINGS PD 890

Serial Number: 008694 Test Record Number: 1574
Test Date: 12/17/2021 Test Time: 12:24pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:24pm
FLO	Pass	12:24pm
FC	Pass	12:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:24pm
SRC	Pass	12:24pm
DET	Pass	12:24pm
BAR	Pass	12:24pm
BT	Pass	12:24pm

Blank Tests

Test	Status	Time
AIR	Pass	12:25pm

Printer Tests


Test	Status	Time
PRNT	Pass	12:25pm

CRC Tests

Test	Status	Time
COMP	Pass	12:25pm
CAL	Pass	12:25pm

Preventive Maintenance

Status: Pass

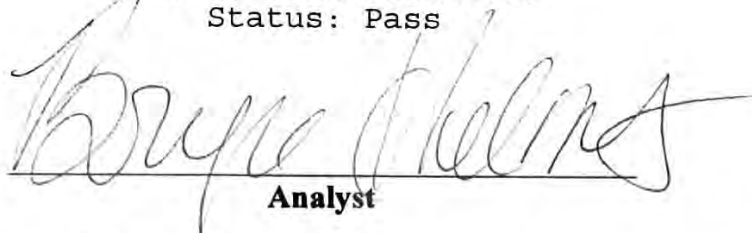

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit C

Instrument Serial No. 008580

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008580
Test Date: 12/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
09/01/2020-09/01/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	9:35pm
AIR BLK	.00	9:36pm
ACCY CHK	.07	9:36pm
AIR BLK	.00	9:37pm
SUB TEST	.00	9:37pm
AIR BLK	.00	9:38pm
SUB TEST	.00	9:40pm
AIR BLK	.00	9:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008580 Test Record Number: 2668
Test Date: 12/18/2021 Test Time: 9:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:42pm
FLO	Pass	9:42pm
FC	Pass	9:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:42pm
SRC	Pass	9:42pm
DET	Pass	9:42pm
BAR	Pass	9:42pm
BT	Pass	9:42pm

Blank Tests

Test	Status	Time
AIR	Pass	9:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:42pm

CRC Tests

Test	Status	Time
COMP	Pass	9:43pm
CAL	Pass	9:43pm

Preventive Maintenance
Status: Pass

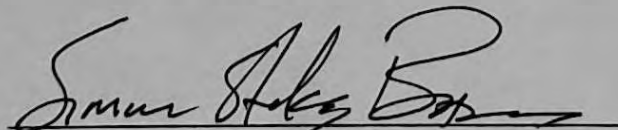
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit 6

Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Erin Adams Bay
Signature of Certifying Official

442
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008584
Test Date: 12/18/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

09/01/2020-09/01/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	10:06pm
AIR BLK	.00	10:07pm
ACCY CHK	.07	10:08pm
AIR BLK	.00	10:09pm
SUB TEST	.00	10:09pm
AIR BLK	.00	10:10pm
SUB TEST	.00	10:12pm
AIR BLK	.00	10:12pm

Reported AC: 100 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008584 Test Record Number: 2411
Test Date: 12/18/2021 Test Time: 10:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:16pm
FLO	Pass	10:16pm
FC	Pass	10:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:17pm
SRC	Pass	10:17pm
DET	Pass	10:17pm
BAR	Pass	10:17pm
BT	Pass	10:17pm

Blank Tests

Test	Status	Time
AIR	Pass	10:17pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:17pm

CRC Tests

Test	Status	Time
COMP	Pass	10:17pm
CAL	Pass	10:17pm

Preventive Maintenance
Status: Pass

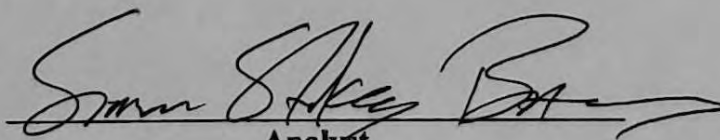
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Cary PD
Instrument Serial No. 008587 120 Wilkeson Ave
Cary, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY CARY PD 910

Serial Number: 008587

Test Date: 12/01/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	4:13pm
AIR BLK	.00	4:14pm
ACCY CHK	.07	4:14pm
AIR BLK	.00	4:15pm
SUB TEST	.00	4:16pm
AIR BLK	.00	4:17pm
SUB TEST	.00	4:18pm
AIR BLK	.00	4:19pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY CARY PD 910

Serial Number: 008587 Test Record Number: 4619
Test Date: 12/01/2021 Test Time: 4:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:20pm
FLO	Pass	4:20pm
FC	Pass	4:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:20pm
SRC	Pass	4:20pm
DET	Pass	4:20pm
BAR	Pass	4:20pm
BT	Pass	4:20pm

Blank Tests

Test	Status	Time
AIR	Pass	4:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:21pm

CRC Tests

Test	Status	Time
COMP	Pass	4:21pm
CAL	Pass	4:21pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT mobile Unit
Instrument Serial No 208601 Knightdale PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008601
Test Date: 12/17/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Smith, Jason R

Permit Number: 0024-7428

Effective:

09/29/2020-09/29/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118805


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	10:11pm
AIR BLK	.00	10:11pm
ACCY CHK	.08	10:12pm
AIR BLK	.00	10:13pm
SUB TEST	.00	10:15pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008601 Test Record Number: 1405
Test Date: 12/17/2021 Test Time: 10:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:21pm
FLO	Pass	10:21pm
FC	Pass	10:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:21pm
SRC	Pass	10:21pm
DET	Pass	10:21pm
BAR	Pass	10:21pm
BT	Pass	10:21pm

Blank Tests

Test	Status	Time
AIR	Pass	10:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:22pm

CRC Tests

Test	Status	Time
COMP	Pass	10:22pm
CAL	Pass	10:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 4
Instrument Serial No. 008601 Raleigh

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

675

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008601
Test Date: 12/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

03/10/2021-03/10/2023

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118805

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	9:49pm
AIR BLK	.00	9:50pm
ACCY CHK	.08	9:51pm
AIR BLK	.00	9:52pm
SUB TEST	.00	9:52pm
AIR BLK	.00	9:53pm
SUB TEST	.00	9:55pm
AIR BLK	.00	9:56pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008601 Test Record Number: 1410
Test Date: 12/18/2021 Test Time: 9:57pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:57pm
FLO	Pass	9:57pm
FC	Pass	9:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:57pm
SRC	Pass	9:57pm
DET	Pass	9:57pm
BAR	Pass	9:57pm
BT	Pass	9:57pm

Blank Tests

Test	Status	Time
AIR	Pass	9:58pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:58pm

CRC Tests

Test	Status	Time
COMP	Pass	9:58pm
CAL	Pass	9:58pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 4
Instrument Serial No. 008615 Raleigh PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008615

Test Date: 12/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Smith, Jason R

Permit Number: 0024-7428

Effective:

09/29/2020-09/29/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018202


Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	11:11pm
AIR BLK	.00	11:12pm
ACCY CHK	.07	11:13pm
AIR BLK	.00	11:14pm
SUB TEST	.00	11:14pm
AIR BLK	.00	11:15pm
SUB TEST	.00	11:17pm
AIR BLK	.00	11:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008615 Test Record Number: 5721
Test Date: 12/18/2021 Test Time: 11:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:19pm
FLO	Pass	11:19pm
FC	Pass	11:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:19pm
SRC	Pass	11:19pm
DET	Pass	11:19pm
BAR	Pass	11:19pm
BT	Pass	11:19pm

Blank Tests

Test	Status	Time
AIR	Pass	11:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:20pm

CRC Tests

Test	Status	Time
COMP	Pass	11:20pm
CAL	Pass	11:20pm

Preventive Maintenance
Status: Pass

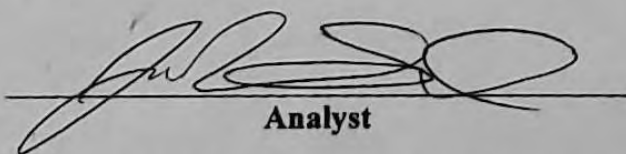

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Apex PD Station 4
Instrument Serial No. 003621 1615 E Williams St
Apex NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of December, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY APEX PD

Serial Number: 008621

Test Date: 12/01/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023


Test	g/210L	Time
DIAG	Pass	2:38pm
AIR BLK	.00	2:39pm
ACCY CHK	.07	2:40pm
AIR BLK	.00	2:41pm
SUB TEST	.00	2:42pm
AIR BLK	.00	2:42pm
SUB TEST	.00	2:44pm
AIR BLK	.00	2:45pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY APEX PD

Serial Number: 008621 Test Record Number: 3140
Test Date: 12/01/2021 Test Time: 2:47pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:47pm
FLO	Pass	2:47pm
FC	Pass	2:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:47pm
SRC	Pass	2:47pm
DET	Pass	2:47pm
BAR	Pass	2:47pm
BT	Pass	2:47pm

Blank Tests

Test	Status	Time
AIR	Pass	2:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:48pm

CRC Tests

Test	Status	Time
COMP	Pass	2:48pm
CAL	Pass	2:48pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 6

Instrument Serial No. 008437

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008637
Test Date: 12/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
09/01/2020-09/01/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG035001
Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	9:58pm
AIR BLK	.00	9:59pm
ACCY CHK	.07	9:59pm
AIR BLK	.00	10:00pm
SUB TEST	.00	10:01pm
AIR BLK	.00	10:02pm
SUB TEST	.00	10:03pm
AIR BLK	.00	10:04pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008637 Test Record Number: 3182
Test Date: 12/18/2021 Test Time: 10:05pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:05pm
FLO	Pass	10:05pm
FC	Pass	10:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:05pm
SRC	Pass	10:05pm
DET	Pass	10:05pm
BAR	Pass	10:05pm
BT	Pass	10:05pm

Blank Tests

Test	Status	Time
AIR	Pass	10:06pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:06pm

CRC Tests

Test	Status	Time
COMP	Pass	10:06pm
CAL	Pass	10:06pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit 6

Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Alan Barnes

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008686
Test Date: 12/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
09/01/2020-09/01/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	9:14pm
AIR BLK	.00	9:15pm
ACCY CHK	.08	9:15pm
AIR BLK	.00	9:16pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:18pm
SUB TEST	.00	9:19pm
AIR BLK	.00	9:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008686 Test Record Number: 6826
Test Date: 12/18/2021 Test Time: 9:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:21pm
FLO	Pass	9:21pm
FC	Pass	9:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:21pm
SRC	Pass	9:21pm
DET	Pass	9:21pm
BAR	Pass	9:21pm
BT	Pass	9:21pm

Blank Tests

Test	Status	Time
AIR	Pass	9:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:22pm

CRC Tests

Test	Status	Time
COMP	Pass	9:22pm
CAL	Pass	9:22pm

Preventive Maintenance
Status: Pass

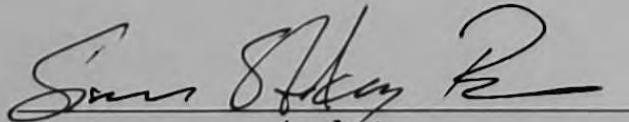
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 4
Instrument Serial No. 008736 Raleigh

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008736

Test Date: 12/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

03/10/2021-03/10/2023

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	9:22pm
AIR BLK	.00	9:23pm
ACCY CHK	.07	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:29pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008736 Test Record Number: 1057
Test Date: 12/18/2021 Test Time: 9:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:30pm
FLO	Pass	9:30pm
FC	Pass	9:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:30pm
SRC	Pass	9:30pm
DET	Pass	9:30pm
BAR	Pass	9:30pm
BT	Pass	9:30pm

Blank Tests

Test	Status	Time
AIR	Pass	9:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:31pm

CRC Tests

Test	Status	Time
COMP	Pass	9:31pm
CAL	Pass	9:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit 6
Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Alex Barron
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008776
Test Date: 12/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

09/01/2020-09/01/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	9:46pm
AIR BLK	.00	9:47pm
ACCY CHK	.07	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:49pm
AIR BLK	.00	9:50pm
SUB TEST	.00	9:51pm
AIR BLK	.00	9:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008776 Test Record Number: 3721
Test Date: 12/18/2021 Test Time: 9:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:53pm
FLO	Pass	9:53pm
FC	Pass	9:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:53pm
SRC	Pass	9:53pm
DET	Pass	9:53pm
BAR	Pass	9:53pm
BT	Pass	9:53pm

Blank Tests

Test	Status	Time
AIR	Pass	9:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:54pm

CRC Tests

Test	Status	Time
COMP	Pass	9:54pm
CAL	Pass	9:54pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 6
Instrument Serial No. 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Samuel Adams Perry
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008779
Test Date: 12/18/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

09/01/2020-09/01/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001


Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	9:24pm
AIR BLK	.00	9:25pm
ACCY CHK	.07	9:26pm
AIR BLK	.00	9:27pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:29pm
SUB TEST	.00	9:30pm
AIR BLK	.00	9:31pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008779 Test Record Number: 3746
Test Date: 12/18/2021 Test Time: 9:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:32pm
FLO	Pass	9:32pm
FC	Pass	9:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:32pm
SRC	Pass	9:32pm
DET	Pass	9:32pm
BAR	Pass	9:32pm
BT	Pass	9:32pm

Blank Tests

Test	Status	Time
AIR	Pass	9:33pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:33pm

CRC Tests

Test	Status	Time
COMP	Pass	9:33pm
CAL	Pass	9:33pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 4
Instrument Serial No. 008929 Raleigh

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

675

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008929
Test Date: 12/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
03/10/2021-03/10/2023

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	9:24pm
AIR BLK	.00	9:25pm
ACCY CHK	.07	9:26pm
AIR BLK	.00	9:27pm
SUB TEST	.00	9:27pm
AIR BLK	.00	9:28pm
SUB TEST	.00	9:30pm
AIR BLK	.00	9:31pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 4 910

Serial Number: 008929 Test Record Number: 1179
Test Date: 12/18/2021 Test Time: 9:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:32pm
FLO	Pass	9:32pm
FC	Pass	9:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:33pm
SRC	Pass	9:33pm
DET	Pass	9:33pm
BAR	Pass	9:33pm
BT	Pass	9:33pm

Blank Tests

Test	Status	Time
AIR	Pass	9:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:33pm

CRC Tests

Test	Status	Time
COMP	Pass	9:34pm
CAL	Pass	9:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wilson Instrument Location Wilson Co Detention Center
Instrument Serial No. 008627 100 E. Green St., Wilson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 6043 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627

Test Date: 12/16/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	10:12am
AIR BLK	.00	10:13am
ACCY CHK	.07	10:13am
AIR BLK	.00	10:14am
SUB TEST	.00	10:15am
AIR BLK	.00	10:16am
SUB TEST	.00	10:17am
AIR BLK	.00	10:18am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627 Test Record Number: 2947
Test Date: 12/16/2021 Test Time: 10:20am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:20am
FLO	Pass	10:20am
FC	Pass	10:20am

Temperature Tests

Test	Status	Time
FC1	Pass	10:21am
SRC	Pass	10:21am
DET	Pass	10:21am
BAR	Pass	10:21am
BT	Pass	10:21am

Blank Tests

Test	Status	Time
AIR	Pass	10:21am


Printer Tests

Test	Status	Time
PRNT	Pass	10:21am

CRC Tests

Test	Status	Time
COMP	Pass	10:21am
CAL	Pass	10:21am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilson Instrument Location Wilson Co Detention Center
Instrument Serial No. 008652 100 E. Green St., Wilson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652
Test Date: 12/16/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	10:26am
AIR BLK	.00	10:27am
ACCY CHK	.08	10:27am
AIR BLK	.00	10:29am
SUB TEST	.00	10:30am
AIR BLK	.00	10:31am
SUB TEST	.00	10:33am
AIR BLK	.00	10:34am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652 Test Record Number: 3602
Test Date: 12/16/2021 Test Time: 10:34am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:35am
FLO	Pass	10:35am
FC	Pass	10:35am

Temperature Tests

Test	Status	Time
FC1	Pass	10:35am
SRC	Pass	10:35am
DET	Pass	10:35am
BAR	Pass	10:35am
BT	Pass	10:35am

Blank Tests

Test	Status	Time
AIR	Pass	10:36am

Printer Tests

Test	Status	Time
PRNT	Pass	10:36am

CRC Tests

Test	Status	Time
COMP	Pass	10:36am
CAL	Pass	10:36am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilson County Instrument Location BAT Mobile Unit 12
Instrument Serial No. 008698 Wilson

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY BAT MOBILE 12 970

Serial Number: 008698

Test Date: 12/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: Unknown

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	8:39pm
AIR BLK	.00	8:40pm
ACCY CHK	.08	8:41pm
AIR BLK	.00	8:42pm
SUB TEST	.00	8:42pm
AIR BLK	.00	8:43pm
SUB TEST	.00	8:45pm
AIR BLK	.00	8:46pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY BAT MOBILE 12 970

Serial Number: 008698 Test Record Number: 1747
Test Date: 12/18/2021 Test Time: 8:47pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:47pm
FLO	Pass	8:47pm
FC	Pass	8:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:47pm
SRC	Pass	8:47pm
DET	Pass	8:47pm
BAR	Pass	8:47pm
BT	Pass	8:47pm

Blank Tests

Test	Status	Time
AIR	Pass	8:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:48pm

CRC Tests

Test	Status	Time
COMP	Pass	8:48pm
CAL	Pass	8:48pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilson County Instrument Location BAT Mobile Unit 12
Instrument Serial No. 008788 Wilson

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY BAT MOBILE UNIT 12 970

Serial Number: 008788
Test Date: 12/18/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	8:26pm
AIR BLK	.00	8:27pm
ACCY CHK	.08	8:28pm
AIR BLK	.00	8:28pm
SUB TEST	.00	8:29pm
AIR BLK	.00	8:30pm
SUB TEST	.00	8:31pm
AIR BLK	.00	8:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY BAT MOBILE UNIT 12 970

Serial Number: 008788 Test Record Number: 1716
Test Date: 12/18/2021 Test Time: 8:34pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:34pm
FLO	Pass	8:35pm
FC	Pass	8:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:35pm
SRC	Pass	8:35pm
DET	Pass	8:35pm
BAR	Pass	8:35pm
BT	Pass	8:35pm

Blank Tests

Test	Status	Time
AIR	Pass	8:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:35pm

CRC Tests

Test	Status	Time
COMP	Pass	8:36pm
CAL	Pass	8:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Yancey Instrument Location Yancey County Jail

Instrument Serial No. 008653 Burnsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 668 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

YANCEY COUNTY YANCEY COUNTY JAIL 990

Serial Number: 008653
Test Date: 12/20/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Loftis, Benjamin C*
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG018401
Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	11:20am
AIR BLK	.00	11:20am
ACCY CHK	.08	11:21am
AIR BLK	.00	11:22am
SUB TEST	.00	11:23am
AIR BLK	.00	11:24am
SUB TEST	.00	11:25am
AIR BLK	.00	11:26am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

YANCEY COUNTY YANCEY COUNTY JAIL 990

Serial Number: 008653 Test Record Number: 1583
Test Date: 12/20/2021 Test Time: 11:26am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:27am
FLO	Pass	11:27am
FC	Pass	11:27am

Temperature Tests

Test	Status	Time
FC1	Pass	11:27am
SRC	Pass	11:27am
DET	Pass	11:27am
BAR	Pass	11:27am
BT	Pass	11:27am

Blank Tests

Test	Status	Time
AIR	Pass	11:28am

Printer Tests

Test	Status	Time
PRNT	Pass	11:28am

CRC Tests

Test	Status	Time
COMP	Pass	11:28am
CAL	Pass	11:28am

Preventive Maintenance
Status: Pass



Analyst