

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 4
Instrument Serial No. 008775 Haw River PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 4 000

Serial Number: 008775
Test Date: 06/19/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Smith, Jason R
Permit Number: 0024-7428
Effective:
09/29/2020-09/29/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	9:26pm
AIR BLK	.00	9:26pm
ACCY CHK	.07	9:27pm
AIR BLK	.00	9:28pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:29pm
SUB TEST	.00	9:31pm
AIR BLK	.00	9:32pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 4 000

Serial Number: 008775 Test Record Number: 1877
Test Date: 06/19/2021 Test Time: 9:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:33pm
FLO	Pass	9:33pm
FC	Pass	9:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:33pm
SRC	Pass	9:33pm
DET	Pass	9:33pm
BAR	Pass	9:33pm
BT	Pass	9:33pm

Blank Tests

Test	Status	Time
AIR	Pass	9:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:34pm

CRC Tests

Test	Status	Time
COMP	Pass	9:34pm
CAL	Pass	9:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location Alamance Co Jail

Instrument Serial No. 008883 109 S Maple St

Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

692
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008853
Test Date: 06/07/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
09/01/2020-09/01/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:00pm
AIR BLK	.00	1:00pm
ACCY CHK	.07	1:01pm
AIR BLK	.00	1:02pm
SUB TEST	.00	1:03pm
AIR BLK	.00	1:04pm
SUB TEST	.00	1:06pm
AIR BLK	.00	1:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008853 Test Record Number: 3403
Test Date: 06/07/2021 Test Time: 1:08pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:09pm
FLO	Pass	1:09pm
FC	Pass	1:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:09pm
SRC	Pass	1:09pm
DET	Pass	1:09pm
BAR	Pass	1:09pm
BT	Pass	1:09pm

Blank Tests

Test	Status	Time
AIR	Pass	1:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:09pm

CRC Tests

Test	Status	Time
COMP	Pass	1:10pm
CAL	Pass	1:10pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alamance Instrument Location Alamance Co Jail

Instrument Serial No. 008913 109 S Maple St

Graham NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913
Test Date: 06/07/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

09/01/2020-09/01/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:01pm
AIR BLK	.00	1:01pm
ACCY CHK	.07	1:02pm
AIR BLK	.00	1:03pm
SUB TEST	.00	1:04pm
AIR BLK	.00	1:05pm
SUB TEST	.00	1:06pm
AIR BLK	.00	1:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913 Test Record Number: 4282
Test Date: 06/07/2021 Test Time: 1:08pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:09pm
FLO	Pass	1:09pm
FC	Pass	1:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:09pm
SRC	Pass	1:09pm
DET	Pass	1:09pm
BAR	Pass	1:09pm
BT	Pass	1:09pm

Blank Tests

Test	Status	Time
AIR	Pass	1:10pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:10pm

CRC Tests

Test	Status	Time
COMP	Pass	1:10pm
CAL	Pass	1:10pm

Preventive Maintenance
Status: Pass

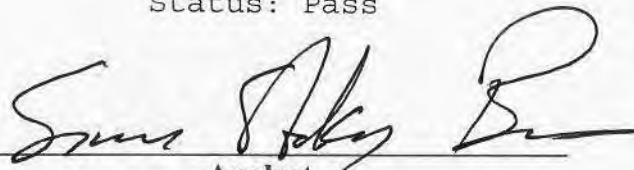

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Allegheny Instrument Location Allegheny Co Jail
Instrument Serial No. 008890 Spartan, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890
Test Date: 06/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: Unknown

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:22am
AIR BLK	.00	12:23am
ACCY CHK	.07	12:24am
AIR BLK	.00	12:25am
SUB TEST	.00	12:25am
AIR BLK	.00	12:26am
SUB TEST	.00	12:28am
AIR BLK	.00	12:28am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890 Test Record Number: 849
Test Date: 06/17/2021 Test Time: 12:29am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:29am
FLO	Pass	12:29am
FC	Pass	12:29am

Temperature Tests

Test	Status	Time
FC1	Pass	12:29am
SRC	Pass	12:29am
DET	Pass	12:29am
BAR	Pass	12:29am
BT	Pass	12:29am

Blank Tests

Test	Status	Time
AIR	Pass	12:30am

Printer Tests

Test	Status	Time
PRNT	Pass	12:30am

CRC Tests

Test	Status	Time
COMP	Pass	12:30am
CAL	Pass	12:30am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Avery Instrument Location Banner Elk PD
Instrument Serial No. 008724 Banner Elk, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724

Test Date: 06/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107502

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	3:51pm
AIR BLK	.00	3:51pm
ACCY CHK	.07	3:52pm
AIR BLK	.00	3:53pm
SUB TEST	.00	3:54pm
AIR BLK	.00	3:55pm
SUB TEST	.00	3:56pm
AIR BLK	.00	3:57pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724 Test Record Number: 672
Test Date: 06/17/2021 Test Time: 3:58pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:58pm
FLO	Pass	3:58pm
FC	Pass	3:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:58pm
SRC	Pass	3:58pm
DET	Pass	3:58pm
BAR	Pass	3:58pm
BT	Pass	3:58pm

Blank Tests

Test	Status	Time
AIR	Pass	3:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:59pm

CRC Tests

Test	Status	Time
COMP	Pass	3:59pm
CAL	Pass	3:59pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Bladen Instrument Location BAT 5 Mobile Unit
Instrument Serial No. 008704 Bladen County Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY BAT MOBILE UNIT 5 080

Serial Number: 008704
Test Date: 06/25/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG807101

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	8:47pm
AIR BLK	.00	8:48pm
ACCY CHK	.08	8:49pm
AIR BLK	.00	8:50pm
SUB TEST	.00	8:50pm
AIR BLK	.00	8:51pm
SUB TEST	.00	8:53pm
AIR BLK	.00	8:54pm

Reported AC: .00 g/210L

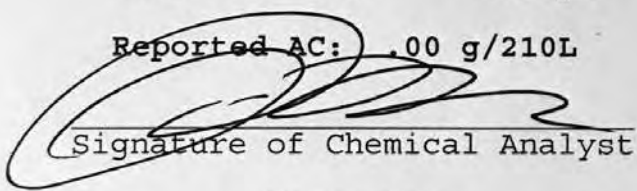
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY BAT MOBILE UNIT 5 080

Serial Number: 008704 Test Record Number: 714
Test Date: 06/25/2021 Test Time: 8:59pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:59pm
FLO	Pass	8:59pm
FC	Pass	8:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:00pm
SRC	Pass	9:00pm
DET	Pass	9:00pm
BAR	Pass	9:00pm
BT	Pass	9:00pm

Blank Tests

Test	Status	Time
AIR	Pass	9:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:00pm

CRC Tests

Test	Status	Time
COMP	Pass	9:00pm
CAL	Pass	9:00pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Buncombe Instrument Location Buncombe Co Jail

Instrument Serial No. 008748 Asheville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BUNCOMBE COUNTY JAIL

100

Serial Number: 008748

Test Date: 06/21/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	1:26pm
AIR BLK	.00	1:26pm
ACCY CHK	.07	1:27pm
AIR BLK	.00	1:28pm
SUB TEST	.00	1:30pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:32pm
AIR BLK	.00	1:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BUNCOMBE COUNTY JAIL 100

Serial Number: 008748 Test Record Number: 1385
Test Date: 06/21/2021 Test Time: 1:40pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:40pm
FLO	Pass	1:40pm
FC	Pass	1:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:40pm
SRC	Pass	1:40pm
DET	Pass	1:40pm
BAR	Pass	1:40pm
BT	Pass	1:40pm

Blank Tests

Test	Status	Time
AIR	Pass	1:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:41pm

CRC Tests

Test	Status	Time
COMP	Pass	1:41pm
CAL	Pass	1:41pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location Buncombe Co. Jail

Instrument Serial No. 003798 Asheville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BUNCOMBE COUNTY JAIL
100

Serial Number: 008798
Test Date: 06/21/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	1:27pm
AIR BLK	.00	1:28pm
ACCY CHK	.08	1:28pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:30pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:33pm
AIR BLK	.00	1:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BUNCOMBE COUNTY JAIL 100

Serial Number: 008798 Test Record Number: 5782
Test Date: 06/21/2021 Test Time: 1:35pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:35pm
FLO	Pass	1:35pm
FC	Pass	1:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:36pm
SRC	Pass	1:36pm
DET	Pass	1:36pm
BAR	Pass	1:36pm
BT	Pass	1:36pm

Blank Tests

Test	Status	Time
AIR	Pass	1:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:36pm

CRC Tests

Test	Status	Time
COMP	Pass	1:36pm
CAL	Pass	1:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Carteret Instrument Location Emerald Isle
Instrument Serial No. 008620 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008620
Test Date: 06/24/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	9:54pm
AIR BLK	.00	9:55pm
ACCY CHK	.07	9:55pm
AIR BLK	.00	9:56pm
SUB TEST	.00	9:57pm
AIR BLK	.00	9:58pm
SUB TEST	.00	9:59pm
AIR BLK	.00	10:00pm

Reported AC: .00 g/210L

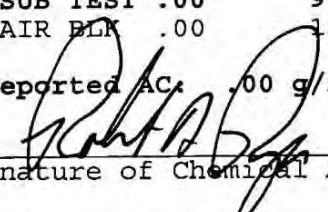

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008620 Test Record Number: 2218
Test Date: 06/24/2021 Test Time: 10:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:03pm
FLO	Pass	10:03pm
FC	Pass	10:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:03pm
SRC	Pass	10:03pm
DET	Pass	10:03pm
BAR	Pass	10:03pm
BT	Pass	10:03pm

Blank Tests

Test	Status	Time
AIR	Pass	10:04pm

Printer Tests


Test	Status	Time
PRNT	Pass	10:04pm

CRC Tests

Test	Status	Time
COMP	Pass	10:04pm
CAL	Pass	10:04pm

Preventive Maintenance

Status: *Pass*

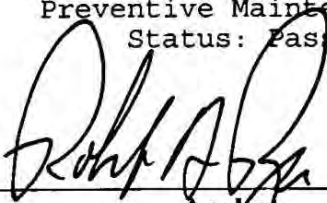

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Carteret Instrument Location Morehead City
Instrument Serial No. 008731 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731

Test Date: 06/24/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	6:10pm
AIR BLK	.00	6:11pm
ACCY CHK	.07	6:12pm
AIR BLK	.00	6:13pm
SUB TEST	.00	6:13pm
AIR BLK	.00	6:14pm
SUB TEST	.00	6:15pm
AIR BLK	.00	6:16pm

Reported As: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731 Test Record Number: 2343
Test Date: 06/24/2021 Test Time: 6:18pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:19pm
FLO	Pass	6:19pm
FC	Pass	6:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:19pm
SRC	Pass	6:19pm
DET	Pass	6:19pm
BAR	Pass	6:19pm
BT	Pass	6:19pm

Blank Tests

Test	Status	Time
AIR	Pass	6:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:20pm

CRC Tests

Test	Status	Time
COMP	Pass	6:20pm
CAL	Pass	6:20pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Carteret Instrument Location Atlantic Beach
Instrument Serial No. 008785 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Robert P. [Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: 008785
Test Date: 06/24/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	8:47pm
AIR BLK	.00	8:48pm
ACCY CHK	.08	8:48pm
AIR BLK	.00	8:49pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:52pm
SUB TEST	.00	8:53pm
AIR BLK	.00	8:54pm

Reported AC: .00 g/210L

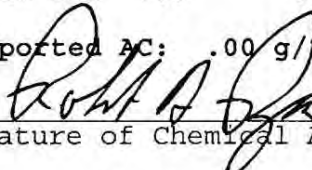

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: 008785 Test Record Number: 1285
Test Date: 06/24/2021 Test Time: 8:56pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:56pm
FLO	Pass	8:56pm
FC	Pass	8:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:56pm
SRC	Pass	8:56pm
DET	Pass	8:56pm
BAR	Pass	8:56pm
BT	Pass	8:56pm

Blank Tests

Test	Status	Time
AIR	Pass	8:57pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:57pm

CRC Tests

Test	Status	Time
COMP	Pass	8:57pm
CAL	Pass	8:57pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Catawba Instrument Location Catawba County SO
Instrument Serial No. 008687 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Hulms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687
Test Date: 06/28/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	12:23pm
AIR BLK	.00	12:23pm
ACCY CHK	.07	12:24pm
AIR BLK	.00	12:25pm
SUB TEST	.00	12:26pm
AIR BLK	.00	12:27pm
SUB TEST	.00	12:28pm
AIR BLK	.00	12:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687 Test Record Number: 3262
Test Date: 06/28/2021 Test Time: 12:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:31pm
FLO	Pass	12:31pm
FC	Pass	12:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:31pm
SRC	Pass	12:31pm
DET	Pass	12:31pm
BAR	Pass	12:31pm
BT	Pass	12:31pm

Blank Tests

Test	Status	Time
AIR	Pass	12:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:32pm

CRC Tests

Test	Status	Time
COMP	Pass	12:32pm
CAL	Pass	12:32pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Catawba Instrument Location Catawba County SO
Instrument Serial No. 008821 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce Hulms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821
Test Date: 06/28/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:19pm
AIR BLK	.00	12:20pm
ACCY CHK	.08	12:20pm
AIR BLK	.00	12:21pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:23pm
SUB TEST	.00	12:24pm
AIR BLK	.00	12:25pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821 Test Record Number: 2192
Test Date: 06/28/2021 Test Time: 12:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:27pm
FLO	Pass	12:27pm
FC	Pass	12:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:27pm
SRC	Pass	12:27pm
DET	Pass	12:27pm
BAR	Pass	12:27pm
BT	Pass	12:27pm

Blank Tests

Test	Status	Time
AIR	Pass	12:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:28pm

CRC Tests

Test	Status	Time
COMP	Pass	12:28pm
CAL	Pass	12:28pm

Preventive Maintenance
Status: Pass

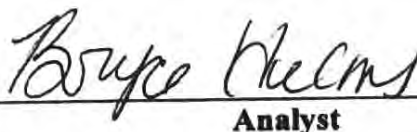

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CHATHAM Instrument Location CHATHAM COUNTY
Instrument Serial No. 008591 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18TH day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008591
Test Date: 06/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	11:57am
AIR BLK	.00	11:57am
ACCY CHK	.08	11:58am
AIR BLK	.00	11:59am
SUB TEST	.00	12:00pm
AIR BLK	.00	12:01pm
SUB TEST	.00	12:02pm
AIR BLK	.00	12:03pm

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008591 Test Record Number: 2540
Test Date: 06/18/2021 Test Time: 12:05pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:06pm
FLO	Pass	12:06pm
FC	Pass	12:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:06pm
SRC	Pass	12:06pm
DET	Pass	12:06pm
BAR	Pass	12:06pm
BT	Pass	12:06pm

Blank Tests

Test	Status	Time
AIR	Pass	12:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:07pm

CRC Tests

Test	Status	Time
COMP	Pass	12:07pm
CAL	Pass	12:07pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CHATHAM Instrument Location SILER CITY
Instrument Serial No. 008811 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18TH day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

6667

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY SILER CITY PD 180

Serial Number: 008811
Test Date: 06/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:56pm
AIR BLK	.00	1:56pm
ACCY CHK	.08	1:57pm
AIR BLK	.00	1:58pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm
SUB TEST	.00	2:01pm
AIR BLK	.00	2:02pm

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY SILER CITY PD 180

Serial Number: 008811 Test Record Number: 1490
Test Date: 06/18/2021 Test Time: 2:04pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:04pm
FLO	Pass	2:04pm
FC	Pass	2:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:04pm
SRC	Pass	2:04pm
DET	Pass	2:04pm
BAR	Pass	2:04pm
BT	Pass	2:04pm

Blank Tests

Test	Status	Time
AIR	Pass	2:05pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:05pm

CRC Tests

Test	Status	Time
COMP	Pass	2:05pm
CAL	Pass	2:05pm

Preventive Maintenance
Status: Pass

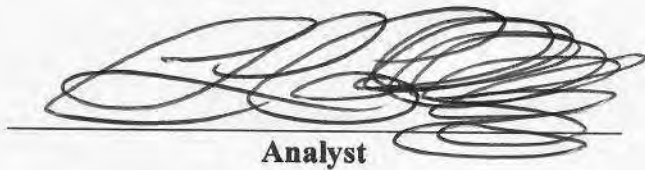

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CHATHAM Instrument Location BAT MODEL UNIT 6

Instrument Serial No. 608590 JORDAN LAKE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY BAT MOBILE UNIT 6 180

Serial Number: 008580
Test Date: 06/27/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

08/14/2019-08/14/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	2:41pm
AIR BLK	.00	2:42pm
ACCY CHK	.07	2:43pm
AIR BLK	.00	2:43pm
SUB TEST	.00	2:44pm
AIR BLK	.00	2:45pm
SUB TEST	.00	2:46pm
AIR BLK	.00	2:47pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY BAT MOBILE UNIT 6 180

Serial Number: 008580 Test Record Number: 2615
Test Date: 06/27/2021 Test Time: 2:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:50pm
FLO	Pass	2:50pm
FC	Pass	2:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:50pm
SRC	Pass	2:50pm
DET	Pass	2:50pm
BAR	Pass	2:50pm
BT	Pass	2:50pm

Blank Tests

Test	Status	Time
AIR	Pass	2:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:50pm

CRC Tests

Test	Status	Time
COMP	Pass	2:51pm
CAL	Pass	2:51pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CHATHAM Instrument Location RAF MORRIS UNIT 6

Instrument Serial No. 008584 JAMAN LANCE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus 2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

463

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY BAT MOBILE UNIT 6 180

Serial Number: 008584
Test Date: 06/27/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

08/14/2019-08/14/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	2:40pm
AIR BLK	.00	2:41pm
ACCY CHK	.07	2:42pm
AIR BLK	.00	2:42pm
SUB TEST	.00	2:43pm
AIR BLK	.00	2:44pm
SUB TEST	.00	2:45pm
AIR BLK	.00	2:46pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY BAT MOBILE UNIT 6 180

Serial Number: 008584 Test Record Number: 2373
Test Date: 06/27/2021 Test Time: 2:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:54pm
FLO	Pass	2:54pm
FC	Pass	2:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:54pm
SRC	Pass	2:54pm
DET	Pass	2:54pm
BAR	Pass	2:54pm
BT	Pass	2:54pm

Blank Tests

Test	Status	Time
AIR	Pass	2:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:55pm

CRC Tests

Test	Status	Time
COMP	Pass	2:55pm
CAL	Pass	2:55pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CHATHAM Instrument Location SAT MODELS UNIT 6

Instrument Serial No. 008686 JONAN LAKE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of JUNE, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

463
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY BAT MOBILE UNIT 6 180

Serial Number: 008686
Test Date: 06/27/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

08/14/2019-08/14/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	2:39pm
AIR BLK	.00	2:40pm
ACCY CHK	.07	2:41pm
AIR BLK	.00	2:42pm
SUB TEST	.00	2:42pm
AIR BLK	.00	2:43pm
SUB TEST	.00	2:45pm
AIR BLK	.00	2:46pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY BAT MOBILE UNIT 6 180

Serial Number: 008686 Test Record Number: 6762
Test Date: 06/27/2021 Test Time: 2:48pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:48pm
FLO	Pass	2:48pm
FC	Pass	2:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:48pm
SRC	Pass	2:48pm
DET	Pass	2:48pm
BAR	Pass	2:48pm
BT	Pass	2:48pm

Blank Tests

Test	Status	Time
AIR	Pass	2:49pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:49pm

CRC Tests

Test	Status	Time
COMP	Pass	2:49pm
CAL	Pass	2:49pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Chowan Instrument Location Chowan Co. Public Safety
Instrument Serial No. 008895 Center, 305 Freemason ST.,
Federton, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Lois Keere 647
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895

Test Date: 06/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Keesler, Linda A

Permit Number: 0045-5468

Effective:

09/16/2020-09/16/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	1:12pm
AIR BLK	.00	1:13pm
ACCY CHK	.07	1:13pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:15pm
AIR BLK	.00	1:16pm
SUB TEST	.00	1:17pm
AIR BLK	.00	1:18pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895 Test Record Number: 1041
Test Date: 06/03/2021 Test Time: 1:19pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:19pm
FLO	Pass	1:19pm
FC	Pass	1:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:20pm
SRC	Pass	1:20pm
DET	Pass	1:20pm
BAR	Pass	1:20pm
BT	Pass	1:20pm

Blank Tests

Test	Status	Time
AIR	Pass	1:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:20pm

CRC Tests

Test	Status	Time
COMP	Pass	1:20pm
CAL	Pass	1:20pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County: Cleveland Instrument Location: Cleveland County SO Annex
Shelby, NC
Instrument Serial No. 008887

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryna Hulms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND ANNEX
220

Serial Number: 00888
Test Date: 06/18/2021

Citation Number: M00000 -0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11 . 19.11
Subject's Sex: Male
Driver's License State:
Driver's License Number: ONE

Analyst's Name: Helms, Br A
Permit Number: 0084-98
Effective:
04/20/2021-04/20/202

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Tes

Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	12: .0m
AIR BLK	.00	12: .0m
ACCY CHK	.08	12: .0m
AIR BLK	.00	12: .0m
SUB TEST	.00	12:25pm
AIR BLK	.00	12: .0m
SUB TEST	.00	12:27pm
AIR BLK	.00	12: .0m

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 8887 Test Record Number: 3448
Test Date: 06/20/11 Test Time: 12:29pm EDT

Self Check: Passed

Baseline Tests

T	Status	Time
I	Pass	12:30pm
F	Pass	12:30pm
F	Pass	12:30pm

Temperature Tests

Temp	Status	Time
FC	Pass	12:30pm
SE	Pass	12:30pm
DE	Pass	12:30pm
BE	Pass	12:30pm
BT	Pass	12:30pm

Blank Tests

Temp	Status	Time
A	Pass	12:31pm

Printer Tests

Temp	Status	Time
P	Pass	12:31pm

CRC Tests

Temp	Status	Time
C	Pass	12:31pm
C	Pass	12:31pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cleveland Instrument Location Cleveland County 80-Annex
Instrument Serial No. 008893 Shelby, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boyer Adams
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008893
Test Date: 06/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
04/20/2021-04/20/2023

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:28pm
AIR BLK	.00	12:29pm
ACCY CHK	.08	12:30pm
AIR BLK	.00	12:31pm
SUB TEST	.00	12:32pm
AIR BLK	.00	12:32pm
SUB TEST	.00	12:34pm
AIR BLK	.00	12:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008893 Test Record Number: 1786
Test Date: 06/18/2021 Test Time: 12:38pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:38pm
FLO	Pass	12:38pm
FC	Pass	12:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:38pm
SRC	Pass	12:38pm
DET	Pass	12:38pm
BAR	Pass	12:38pm
BT	Pass	12:38pm

Blank Tests

Test	Status	Time
AIR	Pass	12:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:39pm

CRC Tests

Test	Status	Time
COMP	Pass	12:39pm
CAL	Pass	12:39pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cleveland Instrument Location Kings Mtn. PD

Instrument Serial No. 008900 Kings Mtn., NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 649 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900
Test Date: 06/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:34am
AIR BLK	.00	10:35am
ACCY CHK	.07	10:35am
AIR BLK	.00	10:37am
SUB TEST	.00	10:37am
AIR BLK	.00	10:38am
SUB TEST	.00	10:40am
AIR BLK	.00	10:40am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900 Test Record Number: 860
Test Date: 06/18/2021 Test Time: 10:41am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:42am
FLO	Pass	10:42am
FC	Pass	10:42am

Temperature Tests

Test	Status	Time
FC1	Pass	10:42am
SRC	Pass	10:42am
DET	Pass	10:42am
BAR	Pass	10:42am
BT	Pass	10:42am

Blank Tests

Test	Status	Time
AIR	Pass	10:42am


Printer Tests

Test	Status	Time
PRNT	Pass	10:43am

CRC Tests

Test	Status	Time
COMP	Pass	10:43am
CAL	Pass	10:43am

Preventive Maintenance
Status: Pass

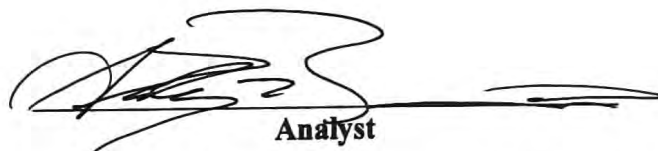

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location Havelock
Instrument Serial No. 008800 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY HAVELOCK PD 240

Serial Number: 008800
Test Date: 06/24/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022


Test	g/210L	Time
DIAG	Pass	4:47pm
AIR BLK	.00	4:48pm
ACCY CHK	.07	4:48pm
AIR BLK	.00	4:49pm
SUB TEST	.00	4:50pm
AIR BLK	.00	4:51pm
SUB TEST	.00	4:52pm
AIR BLK	.00	4:53pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY HAVELOCK PD 240

Serial Number: 008800 Test Record Number: 1415
Test Date: 06/24/2021 Test Time: 4:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:54pm
FLO	Pass	4:54pm
FC	Pass	4:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:54pm
SRC	Pass	4:54pm
DET	Pass	4:54pm
BAR	Pass	4:54pm
BT	Pass	4:54pm

Blank Tests

Test	Status	Time
AIR	Pass	4:55pm

Printer Tests


Test	Status	Time
PRNT	Pass	4:55pm

CRC Tests

Test	Status	Time
COMP	Pass	4:55pm
CAL	Pass	4:55pm

Preventive Maintenance

Status: *Pass*

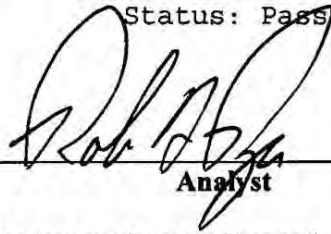

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location New Bern

Instrument Serial No. 008817 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY NEW BERN PD 240

Serial Number: 008817
Test Date: 06/24/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	12:16pm
AIR BLK	.00	12:17pm
ACCY CHK	.07	12:17pm
AIR BLK	.00	12:19pm
SUB TEST	.00	12:19pm
AIR BLK	.00	12:20pm
SUB TEST	.00	12:21pm
AIR BLK	.00	12:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY NEW BERN PD 240

Serial Number: 008817 Test Record Number: 1662
Test Date: 06/24/2021 Test Time: 12:23pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:23pm
FLO	Pass	12:23pm
FC	Pass	12:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:23pm
SRC	Pass	12:23pm
DET	Pass	12:23pm
BAR	Pass	12:23pm
BT	Pass	12:23pm

Blank Tests

Test	Status	Time
AIR	Pass	12:24pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:24pm

CRC Tests

Test	Status	Time
COMP	Pass	12:24pm
CAL	Pass	12:24pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location MCAS

Instrument Serial No. 010819 Cherry Point

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: 010819
Test Date: 06/24/2021

Citation Number: M0000000-0

Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	3:43pm
AIR BLK	.00	3:44pm
ACCY CHK	.07	3:44pm
AIR BLK	.00	3:45pm
SUB TEST	.00	3:46pm
AIR BLK	.00	3:47pm
SUB TEST	.00	3:48pm
AIR BLK	.00	3:49pm

Reported/AC .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: 010819 Test Record Number: 674
Test Date: 06/24/2021 Test Time: 3:50pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:51pm
FLO	Pass	3:51pm
FC	Pass	3:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:51pm
SRC	Pass	3:51pm
DET	Pass	3:51pm
BAR	Pass	3:51pm
BT	Pass	3:51pm

Blank Tests

Test	Status	Time
AIR	Pass	3:51pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:52pm

CRC Tests

Test	Status	Time
COMP	Pass	3:52pm
CAL	Pass	3:52pm

Preventive Maintenance
Status: Pass

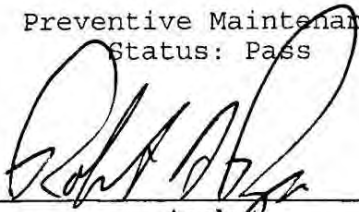

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Currituck Instrument Location Currituck Co. S.O.
Instrument Serial No. 008947 407-A Maple Rd., Maple, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CURRITUCK COUNTY CURRITUCK SO-MAPLE
260

Serial Number: 008947
Test Date: 06/01/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	10:42am
AIR BLK	.00	10:42am
ACCY CHK	.08	10:43am
AIR BLK	.00	10:44am
SUB TEST	.00	10:45am
AIR BLK	.00	10:46am
SUB TEST	.00	10:48am
AIR BLK	.00	10:48am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY CURRITUCK SO-MAPLE 260

Serial Number: 008947 Test Record Number: 2846
Test Date: 06/01/2021 Test Time: 10:50am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:50am
FLO	Pass	10:50am
FC	Pass	10:50am

Temperature Tests

Test	Status	Time
FC1	Pass	10:51am
SRC	Pass	10:51am
DET	Pass	10:51am
BAR	Pass	10:51am
BT	Pass	10:51am

Blank Tests

Test	Status	Time
AIR	Pass	10:51am

Printer Tests

Test	Status	Time
PRNT	Pass	10:51am

CRC Tests

Test	Status	Time
COMP	Pass	10:51am
CAL	Pass	10:51am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Dare Instrument Location Kill Devil Hills P.D.

Instrument Serial No. 008844 107 Town Hall Dr, Kill Devil Hills, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844
Test Date: 06/22/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Guard, Kelly G*
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	4:03pm
AIR BLK	.00	4:04pm
ACCY CHK	.07	4:04pm
AIR BLK	.00	4:06pm
SUB TEST	.00	4:06pm
AIR BLK	.00	4:07pm
SUB TEST	.00	4:09pm
AIR BLK	.00	4:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844 Test Record Number: 2593
Test Date: 06/22/2021 Test Time: 4:10pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:11pm
FLO	Pass	4:11pm
FC	Pass	4:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:11pm
SRC	Pass	4:11pm
DET	Pass	4:11pm
BAR	Pass	4:11pm
BT	Pass	4:11pm

Blank Tests

Test	Status	Time
AIR	Pass	4:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:12pm

CRC Tests

Test	Status	Time
COMP	Pass	4:12pm
CAL	Pass	4:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Duplin Instrument Location Wallace
Instrument Serial No. 008858 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008858
Test Date: 06/21/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	5:03pm
AIR BLK	.00	5:04pm
ACCY CHK	.08	5:04pm
AIR BLK	.00	5:05pm
SUB TEST	.00	5:06pm
AIR BLK	.00	5:07pm
SUB TEST	.00	5:08pm
AIR BLK	.00	5:09pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008858 Test Record Number: 1100
Test Date: 06/21/2021 Test Time: 5:11pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:11pm
FLO	Pass	5:11pm
FC	Pass	5:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:11pm
SRC	Pass	5:11pm
DET	Pass	5:11pm
BAR	Pass	5:11pm
BT	Pass	5:11pm

Blank Tests

Test	Status	Time
AIR	Pass	5:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:12pm

CRC Tests

Test	Status	Time
COMP	Pass	5:12pm
CAL	Pass	5:12pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH CO. DETENTION
Instrument Serial No. 008583 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION

330

Serial Number: 008583

Test Date: 06/22/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107502

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	3:05pm
AIR BLK	.00	3:06pm
ACCY CHK	.08	3:07pm
AIR BLK	.00	3:08pm
SUB TEST	.00	3:08pm
AIR BLK	.00	3:09pm
SUB TEST	.00	3:11pm
AIR BLK	.00	3:12pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008583 Test Record Number: 8462
Test Date: 06/22/2021 Test Time: 3:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:13pm
FLO	Pass	3:13pm
FC	Pass	3:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:14pm
SRC	Pass	3:14pm
DET	Pass	3:14pm
BAR	Pass	3:14pm
BT	Pass	3:14pm

Blank Tests

Test	Status	Time
AIR	Pass	3:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:14pm

CRC Tests

Test	Status	Time
COMP	Pass	3:15pm
CAL	Pass	3:15pm

Preventive Maintenance
Status: Pass

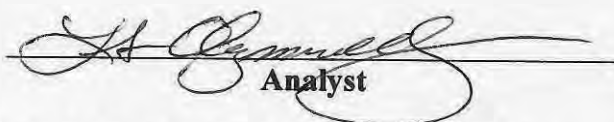
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location KERNERSVILLE

Instrument Serial No. 008650 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650
Test Date: 06/16/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Oligmueller Jr., Leo A*
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933901
Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	3:54pm
AIR BLK	.00	3:56pm
ACCY CHK	.07	3:56pm
AIR BLK	.00	3:57pm
SUB TEST	.00	3:58pm
AIR BLK	.00	3:59pm
SUB TEST	.00	4:01pm
AIR BLK	.00	4:01pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650 Test Record Number: 1788
Test Date: 06/16/2021 Test Time: 4:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:03pm
FLO	Pass	4:03pm
FC	Pass	4:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:03pm
SRC	Pass	4:03pm
DET	Pass	4:03pm
BAR	Pass	4:03pm
BT	Pass	4:03pm

Blank Tests

Test	Status	Time
AIR	Pass	4:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:04pm

CRC Tests

Test	Status	Time
COMP	Pass	4:04pm
CAL	Pass	4:04pm

Preventive Maintenance
Status: Pass

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location FORSYTH CO. DETENTION
Instrument Serial No. 008659 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008659
Test Date: 06/22/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	3:03pm
AIR BLK	.00	3:04pm
ACCY CHK	.08	3:04pm
AIR BLK	.00	3:05pm
SUB TEST	.00	3:06pm
AIR BLK	.00	3:07pm
SUB TEST	.00	3:08pm
AIR BLK	.00	3:09pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008659 Test Record Number: 5729
Test Date: 06/22/2021 Test Time: 3:11pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:11pm
FLO	Pass	3:11pm
FC	Pass	3:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:11pm
SRC	Pass	3:11pm
DET	Pass	3:11pm
BAR	Pass	3:11pm
BT	Pass	3:11pm

Blank Tests

Test	Status	Time
AIR	Pass	3:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:12pm

CRC Tests

Test	Status	Time
COMP	Pass	3:12pm
CAL	Pass	3:12pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Forsyth Instrument Location Forsyth CO Detention
Instrument Serial No. 008925 Winston-Salem, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008925
Test Date: 06/22/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	3:03pm
AIR BLK	.00	3:04pm
ACCY CHK	.08	3:04pm
AIR BLK	.00	3:06pm
SUB TEST	.00	3:06pm
AIR BLK	.00	3:07pm
SUB TEST	.00	3:09pm
AIR BLK	.00	3:10pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008925 Test Record Number: 3786
Test Date: 06/22/2021 Test Time: 3:12pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:12pm
FLO	Pass	3:12pm
FC	Pass	3:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:12pm
SRC	Pass	3:12pm
DET	Pass	3:12pm
BAR	Pass	3:12pm
BT	Pass	3:12pm

Blank Tests

Test	Status	Time
AIR	Pass	3:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:13pm

CRC Tests

Test	Status	Time
COMP	Pass	3:13pm
CAL	Pass	3:13pm

Preventive Maintenance
Status: Pass

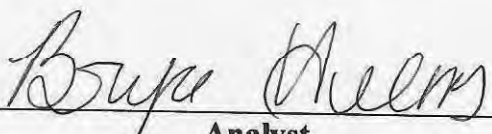

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Franklin Instrument Location Franklin Co LEC

Instrument Serial No. 008733 285 T. Kemp Rd
Louisburg, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008933
Test Date: 06/04/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Bryant Jr., Earl A
Permit Number: 0017-9707
Effective:
09/15/2020-09/15/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	10:10am
AIR BLK	.00	10:11am
ACCY CHK	.07	10:11am
AIR BLK	.00	10:12am
SUB TEST	.00	10:13am
AIR BLK	.00	10:14am
SUB TEST	.00	10:15am
AIR BLK	.00	10:16am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008933 Test Record Number: 1279
Test Date: 06/04/2021 Test Time: 10:18am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:18am
FLO	Pass	10:18am
FC	Pass	10:18am

Temperature Tests

Test	Status	Time
FC1	Pass	10:18am
SRC	Pass	10:18am
DET	Pass	10:18am
BAR	Pass	10:18am
BT	Pass	10:18am

Blank Tests

Test	Status	Time
AIR	Pass	10:19am

Printer Tests

Test	Status	Time
PRNT	Pass	10:19am

CRC Tests

Test	Status	Time
COMP	Pass	10:19am
CAL	Pass	10:19am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Franklin Instrument Location Franklin Co LEC

Instrument Serial No. 008942 285 F Hemp Rd
Louisburg, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. K. [Signature] Signature of Certifying Official 1671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008942
Test Date: 06/04/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Bryant Jr., Earl A
Permit Number: 0017-9707
Effective:
09/15/2020-09/15/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	10:11am
AIR BLK	.00	10:12am
ACCY CHK	.07	10:13am
AIR BLK	.00	10:14am
SUB TEST	.00	10:14am
AIR BLK	.00	10:15am
SUB TEST	.00	10:17am
AIR BLK	.00	10:18am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008942 Test Record Number: 2317
Test Date: 06/04/2021 Test Time: 10:18am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:19am
FLO	Pass	10:19am
FC	Pass	10:19am

Temperature Tests

Test	Status	Time
FC1	Pass	10:19am
SRC	Pass	10:19am
DET	Pass	10:19am
BAR	Pass	10:19am
BT	Pass	10:19am

Blank Tests

Test	Status	Time
AIR	Pass	10:19am


Printer Tests

Test	Status	Time
PRNT	Pass	10:20am

CRC Tests

Test	Status	Time
COMP	Pass	10:20am
CAL	Pass	10:20am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Mt Holly PD
Instrument Serial No. 008733 Mt. Holly, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boye Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY MT. HOLLY PD 350

Serial Number: 008733

Test Date: 06/29/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	10:06am
AIR BLK	.00	10:07am
ACCY CHK	.08	10:08am
AIR BLK	.00	10:08am
SUB TEST	.00	10:09am
AIR BLK	.00	10:10am
SUB TEST	.00	10:11am
AIR BLK	.00	10:12am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY MT. HOLLY PD 350

Serial Number: 008733 Test Record Number: 1269
Test Date: 06/29/2021 Test Time: 10:13am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:13am
FLO	Pass	10:13am
FC	Pass	10:13am

Temperature Tests

Test	Status	Time
FC1	Pass	10:14am
SRC	Pass	10:14am
DET	Pass	10:14am
BAR	Pass	10:14am
BT	Pass	10:14am

Blank Tests

Test	Status	Time
AIR	Pass	10:14am

Printer Tests

Test	Status	Time
PRNT	Pass	10:14am

CRC Tests

Test	Status	Time
COMP	Pass	10:14am
CAL	Pass	10:14am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GRANVILLE Instrument Location BAT MODEL UNIT C
Instrument Serial No. 008637 SLANER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GRANVILLE COUNTY BAT MOBILE UNIT 6 380

Serial Number: 008637
Test Date: 06/25/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

08/14/2019-08/14/2021

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	10:09pm
AIR BLK	.00	10:10pm
ACCY CHK	.07	10:11pm
AIR BLK	.00	10:12pm
SUB TEST	.00	10:12pm
AIR BLK	.00	10:13pm
SUB TEST	.00	10:15pm
AIR BLK	.00	10:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

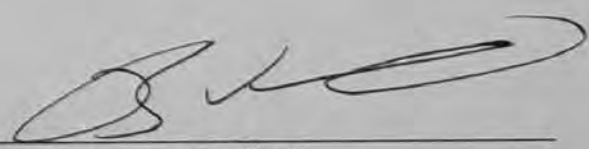

Analyst

Intox EC/IR-II: Preventive Maintenance

GRANVILLE COUNTY BAT MOBILE UNIT 6 380

Serial Number: 008637 Test Record Number: 3117
Test Date: 06/25/2021 Test Time: 10:18pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:19pm
FLO	Pass	10:19pm
FC	Pass	10:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:19pm
SRC	Pass	10:19pm
DET	Pass	10:19pm
BAR	Pass	10:19pm
BT	Pass	10:19pm

Blank Tests

Test	Status	Time
AIR	Pass	10:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:19pm

CRC Tests

Test	Status	Time
COMP	Pass	10:20pm
CAL	Pass	10:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GUILFORD Instrument Location UNC - GREENSBORO

Instrument Serial No. 008604 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY UNC-G POLICE DEPT 400

Serial Number: 008604
Test Date: 06/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: ,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933703
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	10:18am
AIR BLK	.00	10:19am
ACCY CHK	.08	10:20am
AIR BLK	.00	10:21am
SUB TEST	.00	10:22am
AIR BLK	.00	10:23am
SUB TEST	.00	10:24am
AIR BLK	.00	10:25am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY UNC-G POLICE DEPT 400

Serial Number: 008604 Test Record Number: 1970
Test Date: 06/10/2021 Test Time: 10:26am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:26am
FLO	Pass	10:26am
FC	Pass	10:26am

Temperature Tests

Test	Status	Time
FC1	Pass	10:26am
SRC	Pass	10:26am
DET	Pass	10:26am
BAR	Pass	10:26am
BT	Pass	10:26am

Blank Tests

Test	Status	Time
AIR	Pass	10:27am

Printer Tests

Test	Status	Time
PRNT	Pass	10:27am

CRC Tests

Test	Status	Time
COMP	Pass	10:27am
CAL	Pass	10:27am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County GUILFORD Instrument Location GREENSBORO POLICE
Instrument Serial No. 008725 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: 008725
Test Date: 06/30/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107502

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	10:16am
AIR BLK	.00	10:17am
ACCY CHK	.08	10:18am
AIR BLK	.00	10:18am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am
SUB TEST	.00	10:22am
AIR BLK	.00	10:23am

Reported AC: .00 g/210L

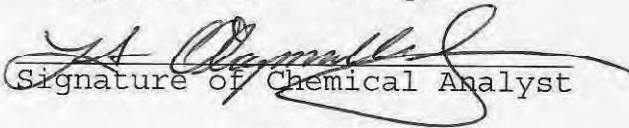
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: 008725 Test Record Number: 4666
Test Date: 06/30/2021 Test Time: 10:24am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:24am
FLO	Pass	10:24am
FC	Pass	10:24am

Temperature Tests

Test	Status	Time
FC1	Pass	10:24am
SRC	Pass	10:24am
DET	Pass	10:24am
BAR	Pass	10:24am
BT	Pass	10:24am

Blank Tests

Test	Status	Time
AIR	Pass	10:25am

Printer Tests

Test	Status	Time
PRNT	Pass	10:25am

CRC Tests

Test	Status	Time
COMP	Pass	10:25am
CAL	Pass	10:25am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Haywood Instrument Location Haywood Co. Jail

Instrument Serial No. 008606 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 668 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008606
Test Date: 06/23/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	1:54pm
AIR BLK	.00	1:55pm
ACCY CHK	.08	1:56pm
AIR BLK	.00	1:56pm
SUB TEST	.00	1:57pm
AIR BLK	.00	1:58pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008606 Test Record Number: 454
Test Date: 06/23/2021 Test Time: 2:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:01pm
FLO	Pass	2:01pm
FC	Pass	2:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:01pm
SRC	Pass	2:01pm
DET	Pass	2:01pm
BAR	Pass	2:01pm
BT	Pass	2:01pm

Blank Tests

Test	Status	Time
AIR	Pass	2:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:02pm

CRC Tests

Test	Status	Time
COMP	Pass	2:02pm
CAL	Pass	2:02pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County HEATFORD Instrument Location Ahoskie P.D.

Instrument Serial No. 008848 705 W. Main St. Ahoskie, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Leila Kest
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848
Test Date: 06/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Keesler, Linda A
Permit Number: 0045-5468
Effective:
09/16/2020-09/16/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	11:41am
AIR BLK	.00	11:41am
ACCY CHK	.07	11:42am
AIR BLK	.00	11:43am
SUB TEST	.00	11:44am
AIR BLK	.00	11:44am
SUB TEST	.00	11:46am
AIR BLK	.00	11:47am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848 Test Record Number: 1602
Test Date: 06/02/2021 Test Time: 11:48am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:48am
FLO	Pass	11:48am
FC	Pass	11:48am

Temperature Tests

Test	Status	Time
FC1	Pass	11:48am
SRC	Pass	11:48am
DET	Pass	11:48am
BAR	Pass	11:48am
BT	Pass	11:48am

Blank Tests

Test	Status	Time
AIR	Pass	11:49am

Printer Tests

Test	Status	Time
PRNT	Pass	11:49am

CRC Tests

Test	Status	Time
COMP	Pass	11:49am
CAL	Pass	11:49am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County HERTFORD Instrument Location Murfreesboro P.D.

Instrument Serial No. 008906 115 E. Broad St., Murfreesboro
N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jina K. Keese
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906
Test Date: 06/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Keesler, Linda A
Permit Number: 0045-5468
Effective:
09/16/2020-09/16/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	12:47pm
AIR BLK	.00	12:48pm
ACCY CHK	.08	12:48pm
AIR BLK	.00	12:49pm
SUB TEST	.00	12:51pm
AIR BLK	.00	12:52pm
SUB TEST	.00	12:53pm
AIR BLK	.00	12:54pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906 Test Record Number: 807
Test Date: 06/02/2021 Test Time: 1:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:03pm
FLO	Pass	1:03pm
FC	Pass	1:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:03pm
SRC	Pass	1:03pm
DET	Pass	1:03pm
BAR	Pass	1:03pm
BT	Pass	1:03pm

Blank Tests

Test	Status	Time
AIR	Pass	1:04pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:04pm

CRC Tests

Test	Status	Time
COMP	Pass	1:04pm
CAL	Pass	1:04pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hyde Instrument Location Hyde Co. SO.

Instrument Serial No. 008801 1233 Main St, Swan Quarter, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801

Test Date: 06/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	10:07am
AIR BLK	.00	10:07am
ACCY CHK	.07	10:08am
AIR BLK	.00	10:09am
SUB TEST	.00	10:09am
AIR BLK	.00	10:10am
SUB TEST	.00	10:12am
AIR BLK	.00	10:13am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801 Test Record Number: 602
Test Date: 06/02/2021 Test Time: 10:13am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:14am
FLO	Pass	10:14am
FC	Pass	10:14am

Temperature Tests

Test	Status	Time
FC1	Pass	10:14am
SRC	Pass	10:14am
DET	Pass	10:14am
BAR	Pass	10:14am
BT	Pass	10:14am

Blank Tests

Test	Status	Time
AIR	Pass	10:15am


Printer Tests

Test	Status	Time
PRNT	Pass	10:15am

CRC Tests

Test	Status	Time
COMP	Pass	10:15am
CAL	Pass	10:15am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County JOHNSTON Instrument Location SELMA POLICE
Instrument Serial No. 008595 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25TH day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595
Test Date: 06/25/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	4:42pm
AIR BLK	.00	4:42pm
ACCY CHK	.07	4:43pm
AIR BLK	.00	4:44pm
SUB TEST	.00	4:45pm
AIR BLK	.00	4:46pm
SUB TEST	.00	4:49pm
AIR BLK	.00	4:50pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595 Test Record Number: 1543
Test Date: 06/25/2021 Test Time: 4:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:51pm
FLO	Pass	4:51pm
FC	Pass	4:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:52pm
SRC	Pass	4:52pm
DET	Pass	4:52pm
BAR	Pass	4:52pm
BT	Pass	4:52pm

Blank Tests

Test	Status	Time
AIR	Pass	4:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:52pm

CRC Tests

Test	Status	Time
COMP	Pass	4:52pm
CAL	Pass	4:52pm

Preventive Maintenance
Status: Pass

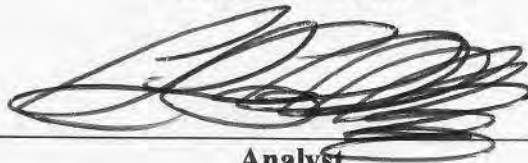

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JOHNSTON Instrument Location CLAYTON POLICE
Instrument Serial No. 008658 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25TH day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY CLAYTON PD 500

Serial Number: 008658
Test Date: 06/25/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	9:52am
AIR BLK	.00	9:53am
ACCY CHK	.08	9:53am
AIR BLK	.00	9:55am
SUB TEST	.00	9:57am
AIR BLK	.00	9:58am
SUB TEST	.00	10:00am
AIR BLK	.00	10:01am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY CLAYTON PD 500

Serial Number: 008658 Test Record Number: 1733
Test Date: 06/25/2021 Test Time: 10:02am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:02am
FLO	Pass	10:02am
FC	Pass	10:02am

Temperature Tests

Test	Status	Time
FC1	Pass	10:02am
SRC	Pass	10:02am
DET	Pass	10:02am
BAR	Pass	10:02am
BT	Pass	10:02am

Blank Tests

Test	Status	Time
AIR	Pass	10:03am

Printer Tests

Test	Status	Time
PRNT	Pass	10:03am

CRC Tests

Test	Status	Time
COMP	Pass	10:03am
CAL	Pass	10:03am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JOHNSTON Instrument Location JOHNSTON COUNTY
Instrument Serial No. 008810 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25TH day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008810

Test Date: 06/25/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	2:36pm
AIR BLK	.00	2:37pm
ACCY CHK	.07	2:38pm
AIR BLK	.00	2:39pm
SUB TEST	.00	2:40pm
AIR BLK	.00	2:40pm
SUB TEST	.00	2:42pm
AIR BLK	.00	2:43pm

Reported AC: .00 g/210L

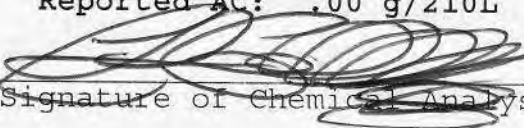
Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008810 Test Record Number: 4544
Test Date: 06/25/2021 Test Time: 2:43pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:44pm
FLO	Pass	2:44pm
FC	Pass	2:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:44pm
SRC	Pass	2:44pm
DET	Pass	2:44pm
BAR	Pass	2:44pm
BT	Pass	2:44pm

Blank Tests

Test	Status	Time
AIR	Pass	2:45pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:45pm

CRC Tests

Test	Status	Time
COMP	Pass	2:45pm
CAL	Pass	2:45pm

Preventive Maintenance
Status: Pass

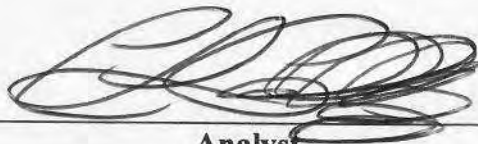

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JOHNSTON Instrument Location JOHNSTON COUNTY
Instrument Serial No. 008846 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25TH day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008846
Test Date: 06/25/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	2:37pm
AIR BLK	.00	2:38pm
ACCY CHK	.07	2:39pm
AIR BLK	.00	2:40pm
SUB TEST	.00	2:40pm
AIR BLK	.00	2:41pm
SUB TEST	.00	2:43pm
AIR BLK	.00	2:44pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008846 Test Record Number: 5471
Test Date: 06/25/2021 Test Time: 2:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:45pm
FLO	Pass	2:45pm
FC	Pass	2:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:46pm
SRC	Pass	2:46pm
DET	Pass	2:46pm
BAR	Pass	2:46pm
BT	Pass	2:46pm

Blank Tests

Test	Status	Time
AIR	Pass	2:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:46pm

CRC Tests

Test	Status	Time
COMP	Pass	2:46pm
CAL	Pass	2:46pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JOHNSTON Instrument Location BENSON POLICE
Instrument Serial No. 008885 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25TH day of JUNE, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BENSON PD 500

Serial Number: 008885

Test Date: 06/25/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034901

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	6:37pm
AIR BLK	.00	6:37pm
ACCY CHK	.08	6:38pm
AIR BLK	.00	6:39pm
SUB TEST	.00	6:39pm
AIR BLK	.00	6:40pm
SUB TEST	.00	6:42pm
AIR BLK	.00	6:42pm

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BENSON PD 500

Serial Number: 008885 Test Record Number: 633
Test Date: 06/25/2021 Test Time: 6:44pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:44pm
FLO	Pass	6:44pm
FC	Pass	6:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:44pm
SRC	Pass	6:44pm
DET	Pass	6:44pm
BAR	Pass	6:44pm
BT	Pass	6:44pm

Blank Tests

Test	Status	Time
AIR	Pass	6:45pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:45pm

CRC Tests

Test	Status	Time
COMP	Pass	6:45pm
CAL	Pass	6:45pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County LEE Instrument Location LEE COUNTY
Instrument Serial No. 008645 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18TH day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY DETENTION CENTER 520

Serial Number: 008645
Test Date: 06/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	4:24pm
AIR BLK	.00	4:24pm
ACCY CHK	.08	4:25pm
AIR BLK	.00	4:26pm
SUB TEST	.00	4:26pm
AIR BLK	.00	4:27pm
SUB TEST	.00	4:29pm
AIR BLK	.00	4:30pm

Reported AC: .00 g/210L

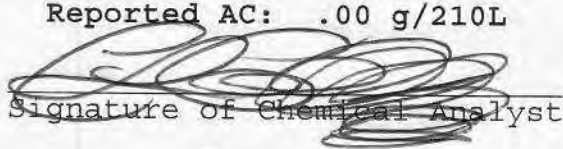
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY DETENTION CENTER 520

Serial Number: 008645 Test Record Number: 2120
Test Date: 06/18/2021 Test Time: 4:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:31pm
FLO	Pass	4:31pm
FC	Pass	4:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:31pm
SRC	Pass	4:31pm
DET	Pass	4:31pm
BAR	Pass	4:31pm
BT	Pass	4:31pm

Blank Tests

Test	Status	Time
AIR	Pass	4:32pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:32pm

CRC Tests

Test	Status	Time
COMP	Pass	4:32pm
CAL	Pass	4:32pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County LEE Instrument Location SANFORD POLICE
Instrument Serial No. 008867 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18TH day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867
Test Date: 06/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	6:03pm
AIR BLK	.00	6:04pm
ACCY CHK	.08	6:04pm
AIR BLK	.00	6:05pm
SUB TEST	.00	6:06pm
AIR BLK	.00	6:07pm
SUB TEST	.00	6:09pm
AIR BLK	.00	6:10pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867 Test Record Number: 1242
Test Date: 06/18/2021 Test Time: 6:11pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:12pm
FLO	Pass	6:12pm
FC	Pass	6:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:12pm
SRC	Pass	6:12pm
DET	Pass	6:12pm
BAR	Pass	6:12pm
BT	Pass	6:12pm

Blank Tests

Test	Status	Time
AIR	Pass	6:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:13pm

CRC Tests

Test	Status	Time
COMP	Pass	6:13pm
CAL	Pass	6:13pm

Preventive Maintenance
Status: Pass

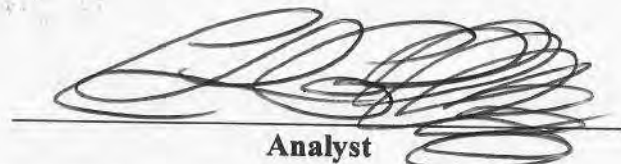

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Lincoln Instrument Location Lincoln Co Courthouse
Instrument Serial No. 008823 Lincolnton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY COURTHOUSE 540

Serial Number: 008823
Test Date: 06/28/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107502

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	10:26am
AIR BLK	.00	10:27am
ACCY CHK	.08	10:28am
AIR BLK	.00	10:29am
SUB TEST	.00	10:29am
AIR BLK	.00	10:30am
SUB TEST	.00	10:32am
AIR BLK	.00	10:33am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY COURTHOUSE 540

Serial Number: 008823 Test Record Number: 1713
Test Date: 06/28/2021 Test Time: 10:33am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:34am
FLO	Pass	10:34am
FC	Pass	10:34am

Temperature Tests

Test	Status	Time
FC1	Pass	10:34am
SRC	Pass	10:34am
DET	Pass	10:34am
BAR	Pass	10:34am
BT	Pass	10:34am

Blank Tests

Test	Status	Time
AIR	Pass	10:35am

Printer Tests

Test	Status	Time
PRNT	Pass	10:35am

CRC Tests

Test	Status	Time
COMP	Pass	10:35am
CAL	Pass	10:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Macon Instrument Location Macon Co. Magistrate

Instrument Serial No. 005795 Highlands, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795
Test Date: 06/09/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, -MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	6:10pm
AIR BLK	.00	6:11pm
ACCY CHK	.08	6:11pm
AIR BLK	.00	6:12pm
SUB TEST	.00	6:13pm
AIR BLK	.00	6:14pm
SUB TEST	.00	6:15pm
AIR BLK	.00	6:16pm

Reported AC: .00 g/210L

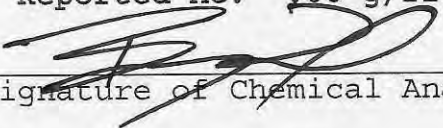

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795 Test Record Number: 538
Test Date: 06/09/2021 Test Time: 6:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:18pm
FLO	Pass	6:18pm
FC	Pass	6:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:18pm
SRC	Pass	6:18pm
DET	Pass	6:18pm
BAR	Pass	6:18pm
BT	Pass	6:18pm

Blank Tests

Test	Status	Time
AIR	Pass	6:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:18pm

CRC Tests

Test	Status	Time
COMP	Pass	6:18pm
CAL	Pass	6:18pm

Preventive Maintenance
Status: Pass

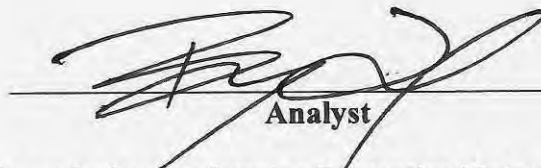

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Madison Instrument Location Madison Co. Jail

Instrument Serial No. 008599 Marshall, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 668 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: 008599

Test Date: 06/21/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	12:03pm
AIR BLK	.00	12:04pm
ACCY CHK	.08	12:04pm
AIR BLK	.00	12:05pm
SUB TEST	.00	12:06pm
AIR BLK	.00	12:06pm
SUB TEST	.00	12:08pm
AIR BLK	.00	12:09pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: 008599 Test Record Number: 1185
Test Date: 06/21/2021 Test Time: 12:09pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:09pm
FLO	Pass	12:09pm
FC	Pass	12:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:10pm
SRC	Pass	12:10pm
DET	Pass	12:10pm
BAR	Pass	12:10pm
BT	Pass	12:10pm

Blank Tests

Test	Status	Time
AIR	Pass	12:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:10pm

CRC Tests

Test	Status	Time
COMP	Pass	12:11pm
CAL	Pass	12:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MARTIN Instrument Location MARTIN CO. S.O.

Instrument Serial No. 008912 305 E. MAIN ST. WILLIAMSTON
N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linna Kase
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912

Test Date: 06/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Keesler, Linda A

Permit Number: 0045-5468

Effective:

09/16/2020-09/16/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:31am
AIR BLK	.00	11:32am
ACCY CHK	.08	11:33am
AIR BLK	.00	11:34am
SUB TEST	.00	11:35am
AIR BLK	.00	11:36am
SUB TEST	.00	11:37am
AIR BLK	.00	11:38am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912 Test Record Number: 1717
Test Date: 06/03/2021 Test Time: 11:47am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:48am
FLO	Pass	11:48am
FC	Pass	11:48am

Temperature Tests

Test	Status	Time
FC1	Pass	11:48am
SRC	Pass	11:48am
DET	Pass	11:48am
BAR	Pass	11:48am
BT	Pass	11:48am

Blank Tests

Test	Status	Time
AIR	Pass	11:48am


Printer Tests

Test	Status	Time
PRNT	Pass	11:48am

CRC Tests

Test	Status	Time
COMP	Pass	11:48am
CAL	Pass	11:48am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County McDowell Instrument Location McDowell Co. Jail

Instrument Serial No. 008999 Marion, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008888

Test Date: 06/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	12:57pm
AIR BLK	.00	12:59pm
ACCY CHK	.07	12:59pm
AIR BLK	.00	1:00pm
SUB TEST	.00	1:01pm
AIR BLK	.00	1:02pm
SUB TEST	.00	1:03pm
AIR BLK	.00	1:04pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008888 Test Record Number: 1599
Test Date: 06/18/2021 Test Time: 1:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:06pm
FLO	Pass	1:06pm
FC	Pass	1:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:06pm
SRC	Pass	1:06pm
DET	Pass	1:06pm
BAR	Pass	1:06pm
BT	Pass	1:06pm

Blank Tests

Test	Status	Time
AIR	Pass	1:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:07pm

CRC Tests

Test	Status	Time
COMP	Pass	1:07pm
CAL	Pass	1:07pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County McDowell Instrument Location McDowell Co Jail
Instrument Serial No. 008592 Marion, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008892
Test Date: 06/18/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:59pm
AIR BLK	.00	1:00pm
ACCY CHK	.07	1:00pm
AIR BLK	.00	1:02pm
SUB TEST	.00	1:02pm
AIR BLK	.00	1:03pm
SUB TEST	.00	1:04pm
AIR BLK	.00	1:05pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008892 Test Record Number: 980
Test Date: 06/18/2021 Test Time: 1:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:06pm
FLO	Pass	1:06pm
FC	Pass	1:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:07pm
SRC	Pass	1:07pm
DET	Pass	1:07pm
BAR	Pass	1:07pm
BT	Pass	1:07pm

Blank Tests

Test	Status	Time
AIR	Pass	1:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:07pm

CRC Tests

Test	Status	Time
COMP	Pass	1:08pm
CAL	Pass	1:08pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County McDowell Instrument Location MOBILE BAT UNIT 2
Instrument Serial No. 008970 Marion

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

673
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL BAT MOBILE UNIT 2 580

Serial Number: 008970
Test Date: 06/11/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barrier II, Dennis J

Permit Number: 0014-7953

Effective:

09/21/2020-09/21/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601


Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	6:08pm
AIR BLK	.00	6:09pm
ACCY CHK	.08	6:10pm
AIR BLK	.00	6:11pm
SUB TEST	.00	6:11pm
AIR BLK	.00	6:12pm
SUB TEST	.00	6:14pm
AIR BLK	.00	6:15pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MCDOWELL BAT MOBILE UNIT 2 580

Serial Number: 008970 Test Record Number: 815
Test Date: 06/11/2021 Test Time: 6:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:16pm
FLO	Pass	6:16pm
FC	Pass	6:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:16pm
SRC	Pass	6:16pm
DET	Pass	6:16pm
BAR	Pass	6:16pm
BT	Pass	6:16pm

Blank Tests

Test	Status	Time
AIR	Pass	6:17pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:17pm

CRC Tests

Test	Status	Time
COMP	Pass	6:17pm
CAL	Pass	6:17pm

Preventive Maintenance
Status: Pass

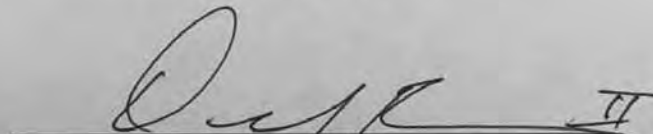

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile unit #5
Instrument Serial No. 008647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 5
590

Serial Number: 008647

Test Date: 06/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	9:30pm
AIR BLK	.00	9:31pm
ACCY CHK	.07	9:32pm
AIR BLK	.00	9:33pm
SUB TEST	.00	9:33pm
AIR BLK	.00	9:34pm
SUB TEST	.00	9:36pm
AIR BLK	.00	9:37pm

Reported AC: .00 g/210L

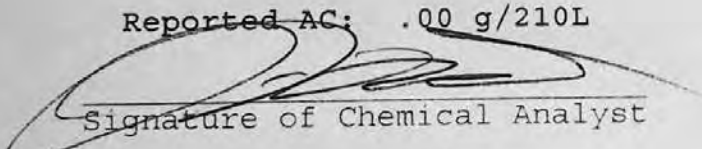
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 5 590
Serial Number: 008647 Test Record Number: 2603
Test Date: 06/17/2021 Test Time: 9:41pm EDT
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:42pm
FLO	Pass	9:42pm
FC	Pass	9:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:42pm
SRC	Pass	9:42pm
DET	Pass	9:42pm
BAR	Pass	9:42pm
BT	Pass	9:42pm

Blank Tests

Test	Status	Time
AIR	Pass	9:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:42pm

CRC Tests

Test	Status	Time
COMP	Pass	9:43pm
CAL	Pass	9:43pm

Preventive Maintenance
Status: Pass

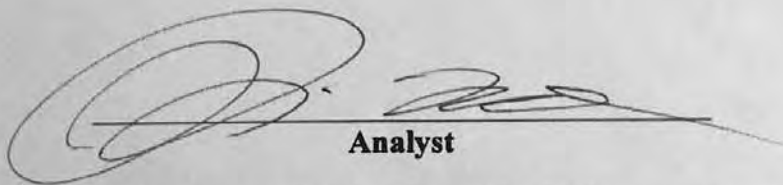

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Cornelius P.D.
Instrument Serial No. 008692 Cornelius, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Adams
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692
Test Date: 06/30/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HELMS, BRYCE A
Permit Number: 0084-9845
Effective:
04/20/2021-04/20/2023

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:24am
AIR BLK	.00	11:25am
ACCY CHK	.07	11:25am
AIR BLK	.00	11:27am
SUB TEST	.00	11:27am
AIR BLK	.00	11:28am
SUB TEST	.00	11:30am
AIR BLK	.00	11:31am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692 Test Record Number: 3127
Test Date: 06/30/2021 Test Time: 11:31am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:32am
FLO	Pass	11:32am
FC	Pass	11:32am

Temperature Tests

Test	Status	Time
FC1	Pass	11:32am
SRC	Pass	11:32am
DET	Pass	11:32am
BAR	Pass	11:32am
BT	Pass	11:32am

Blank Tests

Test	Status	Time
AIR	Pass	11:33am

Printer Tests

Test	Status	Time
PRNT	Pass	11:33am

CRC Tests

Test	Status	Time
COMP	Pass	11:33am
CAL	Pass	11:33am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 4
Instrument Serial No. 008775 NC WRC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted.
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of July, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 4
590

Serial Number: 008775
Test Date: 07/04/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Smith, Jason R

Permit Number: 0024-7428

Effective:

09/29/2020-09/29/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	4:40pm
AIR BLK	.00	4:41pm
ACCY CHK	.07	4:41pm
AIR BLK	.00	4:42pm
SUB TEST	.00	4:43pm
AIR BLK	.00	4:44pm
SUB TEST	.00	4:45pm
AIR BLK	.00	4:46pm

Reported AC: .00 g/210L

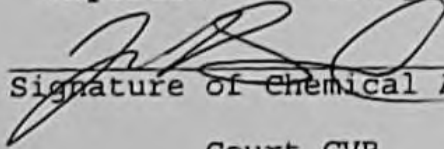
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 4 590

Serial Number: 008775 Test Record Number: 1880
Test Date: 07/04/2021 Test Time: 4:47pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:47pm
FLO	Pass	4:47pm
FC	Pass	4:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:47pm
SRC	Pass	4:47pm
DET	Pass	4:47pm
BAR	Pass	4:47pm
BT	Pass	4:47pm

Blank Tests

Test	Status	Time
AIR	Pass	4:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:48pm

CRC Tests

Test	Status	Time
COMP	Pass	4:48pm
CAL	Pass	4:48pm

Preventive Maintenance
Status: Pass

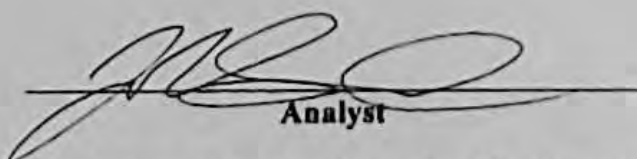
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location Nash Co. Detention Ctr
Instrument Serial No. 213630 2225 Washington St
Nashville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



EABent Signature of Certifying Official 671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY NASH DETENTION CTR 630

Serial Number: 008630
Test Date: 06/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Bryant Jr., Earl A
Permit Number: 0017-9707
Effective:
09/15/2020-09/15/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	2:08pm
AIR BLK	.00	2:09pm
ACCY CHK	.08	2:10pm
AIR BLK	.00	2:11pm
SUB TEST	.00	2:11pm
AIR BLK	.00	2:12pm
SUB TEST	.00	2:13pm
AIR BLK	.00	2:14pm

Reported AC: .00 g/210L

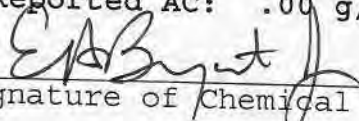
Signature of Chemical Analyst

Court CVR

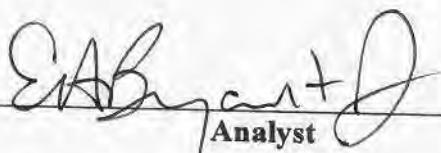
Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY NASH DETENTION CTR 630

Serial Number: 008630 Test Record Number: 5058
Test Date: 06/03/2021 Test Time: 2:15pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:15pm
FLO	Pass	2:15pm
FC	Pass	2:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:15pm
SRC	Pass	2:15pm
DET	Pass	2:15pm
BAR	Pass	2:15pm
BT	Pass	2:15pm

Blank Tests

Test	Status	Time
AIR	Pass	2:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:16pm

CRC Tests

Test	Status	Time
COMP	Pass	2:16pm
CAL	Pass	2:16pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NEW HANOVER Instrument Location WILMINGTON
Instrument Serial No. 008613 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Rg Banes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY WILMINGTON PD 640

Serial Number: 008613

Test Date: 06/21/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Alvin R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	5:09pm
AIR BLK	.00	5:09pm
ACCY CHK	.07	5:10pm
AIR BLK	.00	5:11pm
SUB TEST	.00	5:12pm
AIR BLK	.00	5:12pm
SUB TEST	.00	5:14pm
AIR BLK	.00	5:15pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY WILMINGTON PD 640

Serial Number: 008613 Test Record Number: 1225
Test Date: 06/21/2021 Test Time: 5:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:16pm
FLO	Pass	5:16pm
FC	Pass	5:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:17pm
SRC	Pass	5:17pm
DET	Pass	5:17pm
BAR	Pass	5:17pm
BT	Pass	5:17pm

Blank Tests

Test	Status	Time
AIR	Pass	5:17pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:17pm

CRC Tests

Test	Status	Time
COMP	Pass	5:17pm
CAL	Pass	5:17pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NEW HANOVER Instrument Location NEW HANOVER COUNTY
Instrument Serial No. 008617 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008617
Test Date: 06/23/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	10:17am
AIR BLK	.00	10:18am
ACCY CHK	.07	10:19am
AIR BLK	.00	10:20am
SUB TEST	.00	10:21am
AIR BLK	.00	10:22am
SUB TEST	.00	10:23am
AIR BLK	.00	10:24am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008617 Test Record Number: 3632
Test Date: 06/23/2021 Test Time: 10:25am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:25am
FLO	Pass	10:25am
FC	Pass	10:25am

Temperature Tests

Test	Status	Time
FC1	Pass	10:25am
SRC	Pass	10:25am
DET	Pass	10:25am
BAR	Pass	10:25am
BT	Pass	10:25am

Blank Tests

Test	Status	Time
AIR	Pass	10:26am

Printer Tests

Test	Status	Time
PRNT	Pass	10:26am

CRC Tests

Test	Status	Time
COMP	Pass	10:26am
CAL	Pass	10:26am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NEW HANOVER Instrument Location NEW HANOVER COUNTY
Instrument Serial No. 008626 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Reg Banco
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008626
Test Date: 06/23/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Alvin R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	10:18am
AIR BLK	.00	10:19am
ACCY CHK	.08	10:20am
AIR BLK	.00	10:21am
SUB TEST	.00	10:22am
AIR BLK	.00	10:23am
SUB TEST	.00	10:24am
AIR BLK	.00	10:25am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008626 Test Record Number: 7981
Test Date: 06/23/2021 Test Time: 10:28am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:28am
FLO	Pass	10:28am
FC	Pass	10:28am

Temperature Tests

Test	Status	Time
FC1	Pass	10:29am
SRC	Pass	10:29am
DET	Pass	10:29am
BAR	Pass	10:29am
BT	Pass	10:29am

Blank Tests

Test	Status	Time
AIR	Pass	10:29am

Printer Tests

Test	Status	Time
PRNT	Pass	10:29am

CRC Tests

Test	Status	Time
COMP	Pass	10:29am
CAL	Pass	10:29am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NEW HANOVER Instrument Location CAROLINA BEACH
Instrument Serial No. 008661 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bano
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY CAROLINA BEACH PD
640

Serial Number: 008661
Test Date: 06/23/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Alvin R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902


Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:09pm
AIR BLK	.00	1:10pm
ACCY CHK	.08	1:10pm
AIR BLK	.00	1:11pm
SUB TEST	.00	1:12pm
AIR BLK	.00	1:13pm
SUB TEST	.00	1:14pm
AIR BLK	.00	1:15pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY CAROLINA BEACH PD 640

Serial Number: 008661 Test Record Number: 2808
Test Date: 06/23/2021 Test Time: 1:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:16pm
FLO	Pass	1:16pm
FC	Pass	1:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:16pm
SRC	Pass	1:16pm
DET	Pass	1:16pm
BAR	Pass	1:16pm
BT	Pass	1:16pm

Blank Tests

Test	Status	Time
AIR	Pass	1:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:17pm

CRC Tests

Test	Status	Time
COMP	Pass	1:17pm
CAL	Pass	1:17pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NEW HANOVER Instrument Location WRIGHTSVILLE BEACH
Instrument Serial No. 008667 POLICE DEPT.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bowers
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD
640

Serial Number: 008667
Test Date: 06/23/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	2:40pm
AIR BLK	.00	2:41pm
ACCY CHK	.07	2:42pm
AIR BLK	.00	2:42pm
SUB TEST	.00	2:44pm
AIR BLK	.00	2:45pm
SUB TEST	.00	2:47pm
AIR BLK	.00	2:48pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD 640

Serial Number: 008667 Test Record Number: 2134
Test Date: 06/23/2021 Test Time: 2:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:49pm
FLO	Pass	2:49pm
FC	Pass	2:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:49pm
SRC	Pass	2:49pm
DET	Pass	2:49pm
BAR	Pass	2:49pm
BT	Pass	2:49pm

Blank Tests

Test	Status	Time
AIR	Pass	2:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:50pm

CRC Tests

Test	Status	Time
COMP	Pass	2:50pm
CAL	Pass	2:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location MCAS New River
Instrument Serial No. 008919 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919
Test Date: 06/22/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034901


Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:01pm
AIR BLK	.00	1:02pm
ACCY CHK	.07	1:02pm
AIR BLK	.00	1:04pm
SUB TEST	.00	1:04pm
AIR BLK	.00	1:05pm
SUB TEST	.00	1:07pm
AIR BLK	.00	1:07pm

Reported AC  .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919 Test Record Number: 735
Test Date: 06/22/2021 Test Time: 1:08pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:08pm
FLO	Pass	1:08pm
FC	Pass	1:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:09pm
SRC	Pass	1:09pm
DET	Pass	1:09pm
BAR	Pass	1:09pm
BT	Pass	1:09pm

Blank Tests

Test	Status	Time
AIR	Pass	1:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:09pm

CRC Tests

Test	Status	Time
COMP	Pass	1:09pm
CAL	Pass	1:09pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location Camp LeJeune
Instrument Serial No. 008922 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008922
Test Date: 06/23/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	12:17pm
AIR BLK	.00	12:18pm
ACCY CHK	.07	12:19pm
AIR BLK	.00	12:20pm
SUB TEST	.00	12:21pm
AIR BLK	.00	12:22pm
SUB TEST	.00	12:23pm
AIR BLK	.00	12:24pm

Reported AC: 000 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008922 Test Record Number: 477
Test Date: 06/23/2021 Test Time: 12:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:28pm
FLO	Pass	12:28pm
FC	Pass	12:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:28pm
SRC	Pass	12:28pm
DET	Pass	12:28pm
BAR	Pass	12:28pm
BT	Pass	12:28pm

Blank Tests

Test	Status	Time
AIR	Pass	12:29pm

Printer Tests


Test	Status	Time
PRNT	Pass	12:29pm

CRC Tests

Test	Status	Time
COMP	Pass	12:29pm
CAL	Pass	12:29pm

Preventive Maintenance

Status: *Pass*



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County onslow Instrument Location BAT mobile unit 7

Instrument Serial No. 008969 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008969
Test Date: 06/26/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Anderson, Mark G
Permit Number: 0013-1517
Effective:
09/10/2020-09/10/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	12:23am
AIR BLK	.00	12:24am
ACCY CHK	.08	12:25am
AIR BLK	.00	12:26am
SUB TEST	.00	12:26am
AIR BLK	.00	12:27am
SUB TEST	.00	12:29am
AIR BLK	.00	12:29am

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008969 Test Record Number: 310
Test Date: 06/26/2021 Test Time: 12:32am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:32am
FLO	Pass	12:32am
FC	Pass	12:32am

Temperature Tests

Test	Status	Time
FC1	Pass	12:32am
SRC	Pass	12:32am
DET	Pass	12:32am
BAR	Pass	12:32am
BT	Pass	12:32am

Blank Tests

Test	Status	Time
AIR	Pass	12:33am

Printer Tests

Test	Status	Time
PRNT	Pass	12:33am

CRC Tests

Test	Status	Time
COMP	Pass	12:33am
CAL	Pass	12:33am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location BAT mobile unit 7

Instrument Serial No. 008971 Surf City

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008971
Test Date: 06/19/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Anderson, Mark G
Permit Number: 0013-1517
Effective:
09/10/2020-09/10/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	10:15pm
AIR BLK	.00	10:16pm
ACCY CHK	.07	10:16pm
AIR BLK	.00	10:17pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:20pm
SUB TEST	.00	10:21pm
AIR BLK	.00	10:22pm

Reported AC: .00 g/210L

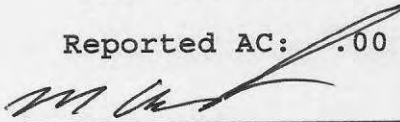

Signature of Chemical Analyst

Court CVR

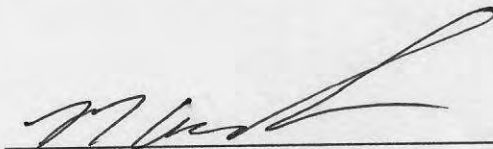

Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008971 Test Record Number: 273
Test Date: 06/19/2021 Test Time: 10:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:24pm
FLO	Pass	10:24pm
FC	Pass	10:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:24pm
SRC	Pass	10:24pm
DET	Pass	10:24pm
BAR	Pass	10:24pm
BT	Pass	10:24pm

Blank Tests

Test	Status	Time
AIR	Pass	10:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:25pm

CRC Tests

Test	Status	Time
COMP	Pass	10:25pm
CAL	Pass	10:25pm

Preventive Maintenance
Status: Pass

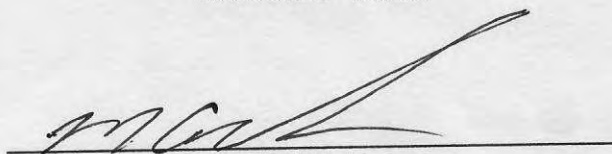

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008972 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008972

Test Date: 06/25/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:33pm
AIR BLK	.00	11:34pm
ACCY CHK	.07	11:35pm
AIR BLK	.00	11:36pm
SUB TEST	.00	11:36pm
AIR BLK	.00	11:37pm
SUB TEST	.00	11:39pm
AIR BLK	.00	11:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008972 Test Record Number: 355
Test Date: 06/25/2021 Test Time: 11:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41pm
FLO	Pass	11:41pm
FC	Pass	11:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:42pm
SRC	Pass	11:42pm
DET	Pass	11:42pm
BAR	Pass	11:42pm
BT	Pass	11:42pm

Blank Tests

Test	Status	Time
AIR	Pass	11:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:42pm

CRC Tests

Test	Status	Time
COMP	Pass	11:42pm
CAL	Pass	11:42pm

Preventive Maintenance
Status: Pass

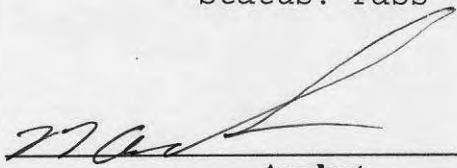

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County onslow Instrument Location BAT mobile unit 7

Instrument Serial No. 008972 surf city

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008972 Test Record Number: 351
Test Date: 06/19/2021 Test Time: 10:31pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:32pm
FLO	Pass	10:32pm
FC	Pass	10:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:32pm
SRC	Pass	10:32pm
DET	Pass	10:32pm
BAR	Pass	10:32pm
BT	Pass	10:32pm

Blank Tests

Test	Status	Time
AIR	Pass	10:33pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:33pm

CRC Tests

Test	Status	Time
COMP	Pass	10:33pm
CAL	Pass	10:33pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008972

Test Date: 06/19/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:16pm
AIR BLK	.00	10:17pm
ACCY CHK	.07	10:17pm
AIR BLK	.00	10:18pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:20pm
SUB TEST	.00	10:21pm
AIR BLK	.00	10:22pm

Reported AC: .00 g/210L

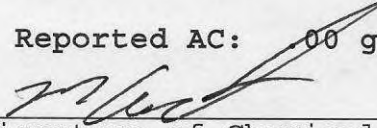

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Orange Instrument Location Cashboro PD

Instrument Serial No. 000651 100 W. Green St. Cashboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 691 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008651
Test Date: 06/28/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Bryant Jr., Earl A
Permit Number: 0017-9707
Effective:
09/15/2020-09/15/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	2:53pm
AIR BLK	.00	2:54pm
ACCY CHK	.08	2:55pm
AIR BLK	.00	2:55pm
SUB TEST	.00	2:56pm
AIR BLK	.00	2:57pm
SUB TEST	.00	2:58pm
AIR BLK	.00	2:59pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008651 Test Record Number: 1504
Test Date: 06/28/2021 Test Time: 3:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:00pm
FLO	Pass	3:00pm
FC	Pass	3:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:00pm
SRC	Pass	3:00pm
DET	Pass	3:00pm
BAR	Pass	3:00pm
BT	Pass	3:00pm

Blank Tests

Test	Status	Time
AIR	Pass	3:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:01pm

CRC Tests

Test	Status	Time
COMP	Pass	3:01pm
CAL	Pass	3:01pm

Preventive Maintenance
Status: Pass

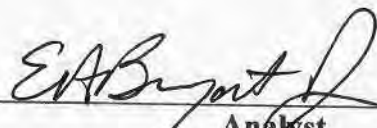

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pamlico Instrument Location Pamlico County
Instrument Serial No. 008640 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PAMLICO COUNTY DETENTION CENTER 680

Serial Number: 008640
Test Date: 06/24/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:50pm
AIR BLK	.00	1:50pm
ACCY CHK	.08	1:51pm
AIR BLK	.00	1:52pm
SUB TEST	.00	1:52pm
AIR BLK	.00	1:53pm
SUB TEST	.00	1:55pm
AIR BLK	.00	1:55pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PAMLICO COUNTY DETENTION CENTER 680

Serial Number: 008640 Test Record Number: 1480
Test Date: 06/24/2021 Test Time: 1:58pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:59pm
FLO	Pass	1:59pm
FC	Pass	1:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:59pm
SRC	Pass	1:59pm
DET	Pass	1:59pm
BAR	Pass	1:59pm
BT	Pass	1:59pm

Blank Tests

Test	Status	Time
AIR	Pass	2:00pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:00pm

CRC Tests

Test	Status	Time
COMP	Pass	2:00pm
CAL	Pass	2:00pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County PENDER Instrument Location PENDER COUNTY
Instrument Serial No. 008946 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Benson
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY DETENTION CENTER 700

Serial Number: 008946
Test Date: 06/28/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	2:45pm
AIR BLK	.00	2:46pm
ACCY CHK	.07	2:46pm
AIR BLK	.00	2:47pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY DETENTION CENTER 700

Serial Number: 008946 Test Record Number: 1192
Test Date: 06/28/2021 Test Time: 2:52pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:52pm
SRC	Pass	2:52pm
DET	Pass	2:52pm
BAR	Pass	2:52pm
BT	Pass	2:52pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:53pm
CAL	Pass	2:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County PENDER Instrument Location PENDER COUNTY
Instrument Serial No. 008948 GOVERNMENT ANNEX

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY GOVERNMENT ANNEX 700

Serial Number: 008948
Test Date: 06/28/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107501
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	11:48am
AIR BLK	.00	11:48am
ACCY CHK	.08	11:49am
AIR BLK	.00	11:50am
SUB TEST	.00	11:51am
AIR BLK	.00	11:51am
SUB TEST	.00	11:53am
AIR BLK	.00	11:54am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY GOVERNMENT ANNEX 700

Serial Number: 008948 Test Record Number: 1143
Test Date: 06/28/2021 Test Time: 11:54am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:55am
FLO	Pass	11:55am
FC	Pass	11:55am

Temperature Tests

Test	Status	Time
FC1	Pass	11:55am
SRC	Pass	11:55am
DET	Pass	11:55am
BAR	Pass	11:55am
BT	Pass	11:55am

Blank Tests

Test	Status	Time
AIR	Pass	11:55am

Printer Tests

Test	Status	Time
PRNT	Pass	11:55am

CRC Tests

Test	Status	Time
COMP	Pass	11:56am
CAL	Pass	11:56am

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County P.H. Instrument Location P.H. Co. Detention Center

Instrument Serial No. 008646 124 New Hope Rd, Greenville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646
Test Date: 06/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	10:50am
AIR BLK	.00	10:51am
ACCY CHK	.08	10:51am
AIR BLK	.00	10:52am
SUB TEST	.00	10:53am
AIR BLK	.00	10:54am
SUB TEST	.00	10:55am
AIR BLK	.00	10:56am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646 Test Record Number: 4243
Test Date: 06/18/2021 Test Time: 10:57am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:58am
FLO	Pass	10:58am
FC	Pass	10:58am

Temperature Tests

Test	Status	Time
FC1	Pass	10:58am
SRC	Pass	10:58am
DET	Pass	10:58am
BAR	Pass	10:58am
BT	Pass	10:58am

Blank Tests

Test	Status	Time
AIR	Pass	10:58am

Printer Tests

Test	Status	Time
PRNT	Pass	10:58am

CRC Tests

Test	Status	Time
COMP	Pass	10:59am
CAL	Pass	10:59am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County P.H. Instrument Location P.H. Co. Detention Center
Instrument Serial No. 008662 129 New Hope Rd, Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1043
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662
Test Date: 06/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Guard, Kelly G
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	11:03am
AIR BLK	.00	11:04am
ACCY CHK	.08	11:05am
AIR BLK	.00	11:06am
SUB TEST	.00	11:06am
AIR BLK	.00	11:07am
SUB TEST	.00	11:09am
AIR BLK	.00	11:10am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662 Test Record Number: 1217
Test Date: 06/18/2021 Test Time: 11:11am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:12am
FLO	Pass	11:12am
FC	Pass	11:12am

Temperature Tests

Test	Status	Time
FC1	Pass	11:12am
SRC	Pass	11:12am
DET	Pass	11:12am
BAR	Pass	11:12am
BT	Pass	11:12am

Blank Tests

Test	Status	Time
AIR	Pass	11:13am


Printer Tests

Test	Status	Time
PRNT	Pass	11:13am

CRC Tests

Test	Status	Time
COMP	Pass	11:13am
CAL	Pass	11:13am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Polk Instrument Location Polk County Jail

Instrument Serial No. 008852 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY LEC 740

Serial Number: 008832
Test Date: 06/22/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:02pm
AIR BLK	.00	1:03pm
ACCY CHK	.07	1:04pm
AIR BLK	.00	1:05pm
SUB TEST	.00	1:06pm
AIR BLK	.00	1:07pm
SUB TEST	.00	1:08pm
AIR BLK	.00	1:09pm

Reported AC: .00 g/210L

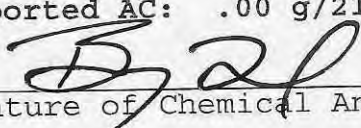

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY LEC 740

Serial Number: 008832 Test Record Number: 1626
Test Date: 06/22/2021 Test Time: 1:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:21pm
FLO	Pass	1:21pm
FC	Pass	1:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:22pm
SRC	Pass	1:22pm
DET	Pass	1:22pm
BAR	Pass	1:22pm
BT	Pass	1:22pm

Blank Tests

Test	Status	Time
AIR	Pass	1:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:22pm

CRC Tests

Test	Status	Time
COMP	Pass	1:23pm
CAL	Pass	1:23pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Polk Instrument Location Polk County Jail

Instrument Serial No. 008981 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 1668 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY LEC 740

Serial Number: 008881
Test Date: 06/22/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018401
Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	1:04pm
AIR BLK	.00	1:05pm
ACCY CHK	.08	1:06pm
AIR BLK	.00	1:07pm
SUB TEST	.00	1:08pm
AIR BLK	.00	1:08pm
SUB TEST	.00	1:10pm
AIR BLK	.00	1:11pm

Reported AC: .00 g/210L

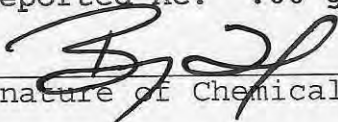

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY LEC 740

Serial Number: 008881 Test Record Number: 966
Test Date: 06/22/2021 Test Time: 1:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:13pm
FLO	Pass	1:13pm
FC	Pass	1:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:13pm
SRC	Pass	1:13pm
DET	Pass	1:13pm
BAR	Pass	1:13pm
BT	Pass	1:13pm

Blank Tests

Test	Status	Time
AIR	Pass	1:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:14pm

CRC Tests

Test	Status	Time
COMP	Pass	1:14pm
CAL	Pass	1:14pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County RANDOLPH Instrument Location RANDOLPH CO. DETENTION CENTER
Instrument Serial No. 008860 ASHEBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: 008860

Test Date: 06/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	9:00am
AIR BLK	.00	9:01am
ACCY CHK	.07	9:01am
AIR BLK	.00	9:02am
SUB TEST	.00	9:03am
AIR BLK	.00	9:04am
SUB TEST	.00	9:06am
AIR BLK	.00	9:06am

Reported AC: .00 g/210L

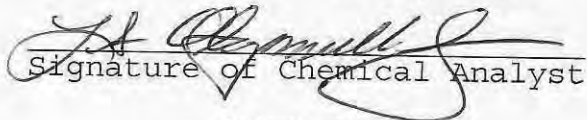
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: 008860 Test Record Number: 2987
Test Date: 06/18/2021 Test Time: 9:09am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:09am
FLO	Pass	9:09am
FC	Pass	9:10am

Temperature Tests

Test	Status	Time
FC1	Pass	9:10am
SRC	Pass	9:10am
DET	Pass	9:10am
BAR	Pass	9:10am
BT	Pass	9:10am

Blank Tests

Test	Status	Time
AIR	Pass	9:10am


Printer Tests

Test	Status	Time
PRNT	Pass	9:10am

CRC Tests

Test	Status	Time
COMP	Pass	9:11am
CAL	Pass	9:11am

Preventive Maintenance
Status: Pass

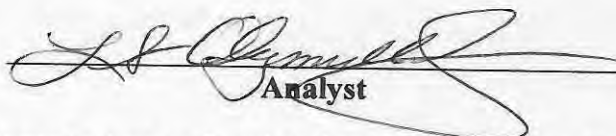
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RANDOLPH Instrument Location RANDOLPH CO. DETENTION CENTER
Instrument Serial No. 008899 ASHEBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: 008899
Test Date: 06/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	9:01am
AIR BLK	.00	9:02am
ACCY CHK	.08	9:03am
AIR BLK	.00	9:04am
SUB TEST	.00	9:04am
AIR BLK	.00	9:05am
SUB TEST	.00	9:07am
AIR BLK	.00	9:08am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: 008899 Test Record Number: 3631
Test Date: 06/18/2021 Test Time: 9:09am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:09am
FLO	Pass	9:09am
FC	Pass	9:09am

Temperature Tests

Test	Status	Time
FC1	Pass	9:09am
SRC	Pass	9:09am
DET	Pass	9:09am
BAR	Pass	9:09am
BT	Pass	9:09am

Blank Tests

Test	Status	Time
AIR	Pass	9:10am

Printer Tests

Test	Status	Time
PRNT	Pass	9:10am

CRC Tests

Test	Status	Time
COMP	Pass	9:10am
CAL	Pass	9:10am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BATS Mobile Unit
Instrument Serial No. 008616 NCSHP

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008616
Test Date: 06/26/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Todd, Shane C
Permit Number: 0035-4789
Effective:
10/06/2020-10/06/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933703
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	7:31pm
AIR BLK	.00	7:32pm
ACCY CHK	.07	7:33pm
AIR BLK	.00	7:34pm
SUB TEST	.00	7:34pm
AIR BLK	.00	7:35pm
SUB TEST	.00	7:37pm
AIR BLK	.00	7:38pm

Reported AC: .00 g/210L

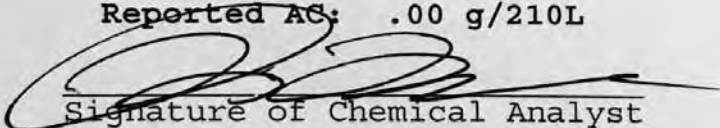
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008616 Test Record Number: 2613
Test Date: 06/26/2021 Test Time: 7:42pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	7:42pm
FLO	Pass	7:42pm
FC	Pass	7:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:42pm
SRC	Pass	7:42pm
DET	Pass	7:42pm
BAR	Pass	7:42pm
BT	Pass	7:42pm

Blank Tests

Test	Status	Time
AIR	Pass	7:43pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:43pm

CRC Tests

Test	Status	Time
COMP	Pass	7:43pm
CAL	Pass	7:43pm

Preventive Maintenance
Status: Pass

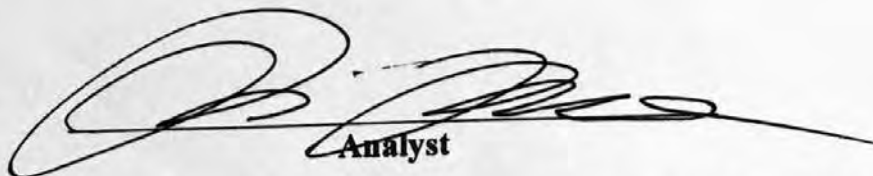
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROBESON Instrument Location ST. PAULS
Instrument Serial No. 008814 POLICE DEPT.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21ST day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY ST PAULS PD 770

Serial Number: 008814

Test Date: 06/21/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	4:11pm
AIR BLK	.00	4:12pm
ACCY CHK	.08	4:12pm
AIR BLK	.00	4:14pm
SUB TEST	.00	4:14pm
AIR BLK	.00	4:15pm
SUB TEST	.00	4:17pm
AIR BLK	.00	4:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY ST PAULS PD 770

Serial Number: 008814 Test Record Number: 752
Test Date: 06/21/2021 Test Time: 4:18pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:19pm
FLO	Pass	4:19pm
FC	Pass	4:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:19pm
SRC	Pass	4:19pm
DET	Pass	4:19pm
BAR	Pass	4:19pm
BT	Pass	4:19pm

Blank Tests

Test	Status	Time
AIR	Pass	4:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:20pm

CRC Tests

Test	Status	Time
COMP	Pass	4:20pm
CAL	Pass	4:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT 5 Mobile Unit
Instrument Serial No. 008826 NC5HP

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826
Test Date: 06/26/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG934303

Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	7:30pm
AIR BLK	.00	7:31pm
ACCY CHK	.08	7:31pm
AIR BLK	.00	7:32pm
SUB TEST	.00	7:33pm
AIR BLK	.00	7:33pm
SUB TEST	.00	7:35pm
AIR BLK	.00	7:36pm

Reported AC: .00 g/210L

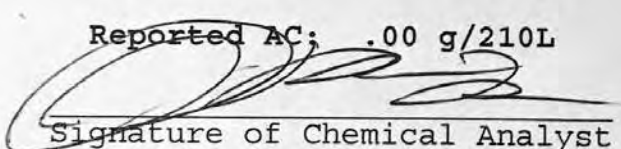
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826 Test Record Number: 8323
Test Date: 06/26/2021 Test Time: 7:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:37pm
FLO	Pass	7:37pm
FC	Pass	7:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:37pm
SRC	Pass	7:37pm
DET	Pass	7:37pm
BAR	Pass	7:37pm
BT	Pass	7:37pm

Blank Tests

Test	Status	Time
AIR	Pass	7:38pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:38pm

CRC Tests

Test	Status	Time
COMP	Pass	7:38pm
CAL	Pass	7:38pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROCKINGHAM Instrument Location ROCKINGHAM COUNTY JAIL
Instrument Serial No. 008796 WENTWORTH, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL
780

Serial Number: 008796
Test Date: 06/28/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:07pm
AIR BLK	.00	1:08pm
ACCY CHK	.08	1:08pm
AIR BLK	.00	1:09pm
SUB TEST	.00	1:10pm
AIR BLK	.00	1:11pm
SUB TEST	.00	1:12pm
AIR BLK	.00	1:13pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL 780

Serial Number: 008796 Test Record Number: 3148
Test Date: 06/28/2021 Test Time: 1:14pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:14pm
FLO	Pass	1:14pm
FC	Pass	1:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:15pm
SRC	Pass	1:15pm
DET	Pass	1:15pm
BAR	Pass	1:15pm
BT	Pass	1:15pm

Blank Tests

Test	Status	Time
AIR	Pass	1:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:15pm

CRC Tests

Test	Status	Time
COMP	Pass	1:15pm
CAL	Pass	1:15pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCI

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROCKINGHAM Instrument Location MADISON POLICE

Instrument Serial No. 008802 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY MADISON PD 780

Serial Number: 008802
Test Date: 06/28/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	2:35pm
AIR BLK	.00	2:36pm
ACCY CHK	.08	2:37pm
AIR BLK	.00	2:37pm
SUB TEST	.00	2:38pm
AIR BLK	.00	2:39pm
SUB TEST	.00	2:40pm
AIR BLK	.00	2:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY MADISON PD 780

Serial Number: 008802 Test Record Number: 914
Test Date: 06/28/2021 Test Time: 2:42pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:43pm
FLO	Pass	2:43pm
FC	Pass	2:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:43pm
SRC	Pass	2:43pm
DET	Pass	2:43pm
BAR	Pass	2:43pm
BT	Pass	2:43pm

Blank Tests

Test	Status	Time
AIR	Pass	2:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:43pm

CRC Tests

Test	Status	Time
COMP	Pass	2:44pm
CAL	Pass	2:44pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROWAN Instrument Location SALISBURY POLICE

Instrument Serial No. 008868 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868
Test Date: 06/17/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Oligmueller Jr., Leo A*
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933703
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	7:50am
AIR BLK	.00	7:50am
ACCY CHK	.08	7:51am
AIR BLK	.00	7:52am
SUB TEST	.00	7:53am
AIR BLK	.00	7:54am
SUB TEST	.00	7:55am
AIR BLK	.00	7:56am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868 Test Record Number: 3235
Test Date: 06/17/2021 Test Time: 7:57am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:57am
FLO	Pass	7:57am
FC	Pass	7:57am

Temperature Tests

Test	Status	Time
FC1	Pass	7:58am
SRC	Pass	7:58am
DET	Pass	7:58am
BAR	Pass	7:58am
BT	Pass	7:58am

Blank Tests

Test	Status	Time
AIR	Pass	7:58am

Printer Tests

Test	Status	Time
PRNT	Pass	7:58am

CRC Tests

Test	Status	Time
COMP	Pass	7:58am
CAL	Pass	7:58am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Rutherford Instrument Location Forest City Police Dept

Instrument Serial No. 008889 Forest City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: 008889
Test Date: 06/22/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:33am
AIR BLK	.00	11:34am
ACCY CHK	.07	11:35am
AIR BLK	.00	11:36am
SUB TEST	.00	11:37am
AIR BLK	.00	11:38am
SUB TEST	.00	11:39am
AIR BLK	.00	11:40am

Reported AC: .00 g/210L

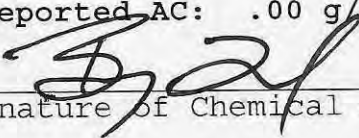

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: 008889 Test Record Number: 949
Test Date: 06/22/2021 Test Time: 11:41am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41am
FLO	Pass	11:41am
FC	Pass	11:41am

Temperature Tests

Test	Status	Time
FC1	Pass	11:41am
SRC	Pass	11:41am
DET	Pass	11:41am
BAR	Pass	11:41am
BT	Pass	11:41am

Blank Tests

Test	Status	Time
AIR	Pass	11:42am

Printer Tests

Test	Status	Time
PRNT	Pass	11:42am

CRC Tests

Test	Status	Time
COMP	Pass	11:42am
CAL	Pass	11:42am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Rutherford Instrument Location Rutherford Co Jail

Instrument Serial No. 008914 Rutherfordton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY RUTHERFORD COUNTY SO
800

Serial Number: 008914
Test Date: 06/22/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG934303

Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	2:26pm
AIR BLK	.00	2:26pm
ACCY CHK	.08	2:27pm
AIR BLK	.00	2:28pm
SUB TEST	.00	2:29pm
AIR BLK	.00	2:29pm
SUB TEST	.00	2:31pm
AIR BLK	.00	2:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY RUTHERFORD COUNTY SO 800

Serial Number: 008914 Test Record Number: 2309
Test Date: 06/22/2021 Test Time: 2:32pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:32pm
FLO	Pass	2:32pm
FC	Pass	2:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:33pm
SRC	Pass	2:33pm
DET	Pass	2:33pm
BAR	Pass	2:33pm
BT	Pass	2:33pm

Blank Tests

Test	Status	Time
AIR	Pass	2:33pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:33pm

CRC Tests

Test	Status	Time
COMP	Pass	2:33pm
CAL	Pass	2:33pm

Preventive Maintenance
Status: Pass

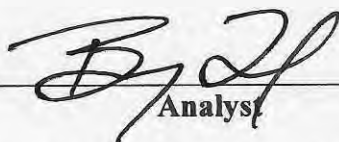
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County SAMPSON Instrument Location SAMPSON COUNTY
Instrument Serial No. 008825 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bano

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825
Test Date: 06/16/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	4:23pm
AIR BLK	.00	4:23pm
ACCY CHK	.07	4:24pm
AIR BLK	.00	4:25pm
SUB TEST	.00	4:25pm
AIR BLK	.00	4:26pm
SUB TEST	.00	4:28pm
AIR BLK	.00	4:29pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825 Test Record Number: 3212
Test Date: 06/16/2021 Test Time: 4:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:30pm
FLO	Pass	4:30pm
FC	Pass	4:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:30pm
SRC	Pass	4:30pm
DET	Pass	4:30pm
BAR	Pass	4:30pm
BT	Pass	4:30pm

Blank Tests

Test	Status	Time
AIR	Pass	4:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:31pm

CRC Tests

Test	Status	Time
COMP	Pass	4:31pm
CAL	Pass	4:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County SAMPSON Instrument Location SAMPSON COUNTY
Instrument Serial No. 008877 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877

Test Date: 06/16/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Alvin R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034901

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	4:14pm
AIR BLK	.00	4:15pm
ACCY CHK	.08	4:16pm
AIR BLK	.00	4:17pm
SUB TEST	.00	4:17pm
AIR BLK	.00	4:18pm
SUB TEST	.00	4:20pm
AIR BLK	.00	4:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877 Test Record Number: 3417
Test Date: 06/16/2021 Test Time: 4:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:21pm
FLO	Pass	4:21pm
FC	Pass	4:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:21pm
SRC	Pass	4:21pm
DET	Pass	4:21pm
BAR	Pass	4:21pm
BT	Pass	4:21pm

Blank Tests

Test	Status	Time
AIR	Pass	4:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:22pm

CRC Tests

Test	Status	Time
COMP	Pass	4:22pm
CAL	Pass	4:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County STOKES Instrument Location STOKES COUNTY JAIL

Instrument Serial No. 008596 DANBURY, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596

Test Date: 06/14/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	9:32am
AIR BLK	.00	9:33am
ACCY CHK	.07	9:33am
AIR BLK	.00	9:34am
SUB TEST	.00	9:35am
AIR BLK	.00	9:36am
SUB TEST	.00	9:37am
AIR BLK	.00	9:38am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596 Test Record Number: 1191
Test Date: 06/14/2021 Test Time: 9:39am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:40am
FLO	Pass	9:40am
FC	Pass	9:40am

Temperature Tests

Test	Status	Time
FC1	Pass	9:40am
SRC	Pass	9:40am
DET	Pass	9:40am
BAR	Pass	9:40am
BT	Pass	9:40am

Blank Tests

Test	Status	Time
AIR	Pass	9:40am

Printer Tests

Test	Status	Time
PRNT	Pass	9:40am

CRC Tests

Test	Status	Time
COMP	Pass	9:41am
CAL	Pass	9:41am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Surry Instrument Location Elkin Police
Instrument Serial No. 008926 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY ELKIN PD 850

Serial Number: 008926
Test Date: 06/10/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male

Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J
Permit Number: 0018-4401
Effective:
10/01/2020-10/01/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	6:34pm
AIR BLK	.00	6:35pm
ACCY CHK	.08	6:36pm
AIR BLK	.00	6:37pm
SUB TEST	.00	6:37pm
AIR BLK	.00	6:38pm
SUB TEST	.00	6:40pm
AIR BLK	.00	6:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY ELKIN PD 850

Serial Number: 008926 Test Record Number: 977
Test Date: 06/10/2021 Test Time: 6:44pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:44pm
FLO	Pass	6:44pm
FC	Pass	6:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:44pm
SRC	Pass	6:44pm
DET	Pass	6:44pm
BAR	Pass	6:44pm
BT	Pass	6:44pm

Blank Tests

Test	Status	Time
AIR	Pass	6:45pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:45pm

CRC Tests

Test	Status	Time
COMP	Pass	6:45pm
CAL	Pass	6:45pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Surry Instrument Location Mount Airy
Instrument Serial No. 008443 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

689
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943
Test Date: 06/08/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: Unknown

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	7:35pm
AIR BLK	.00	7:35pm
ACCY CHK	.07	7:36pm
AIR BLK	.00	7:37pm
SUB TEST	.00	7:38pm
AIR BLK	.00	7:38pm
SUB TEST	.00	7:40pm
AIR BLK	.00	7:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943 Test Record Number: 2297
Test Date: 06/08/2021 Test Time: 7:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:42pm
FLO	Pass	7:42pm
FC	Pass	7:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:42pm
SRC	Pass	7:42pm
DET	Pass	7:42pm
BAR	Pass	7:42pm
BT	Pass	7:42pm

Blank Tests

Test	Status	Time
AIR	Pass	7:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:43pm

CRC Tests

Test	Status	Time
COMP	Pass	7:43pm
CAL	Pass	7:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Union Instrument Location Waxhaw PD
Instrument Serial No. 008598 Waxhaw, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY WAXHAW PD 890

Serial Number: 008598

Test Date: 06/29/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAITENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	2:33pm
AIR BLK	.00	2:33pm
ACCY CHK	.07	2:34pm
AIR BLK	.00	2:35pm
SUB TEST	.00	2:36pm
AIR BLK	.00	2:37pm
SUB TEST	.00	2:38pm
AIR BLK	.00	2:39pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY WAXHAW PD 890

Serial Number: 008598 Test Record Number: 879
Test Date: 06/29/2021 Test Time: 2:40pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:40pm
FLO	Pass	2:40pm
FC	Pass	2:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:40pm
SRC	Pass	2:40pm
DET	Pass	2:40pm
BAR	Pass	2:40pm
BT	Pass	2:40pm

Blank Tests

Test	Status	Time
AIR	Pass	2:41pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:41pm

CRC Tests

Test	Status	Time
COMP	Pass	2:41pm
CAL	Pass	2:41pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT mobile Unit 1

Instrument Serial No. 008895 Apex 10

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 1 910

Serial Number: 008898
Test Date: 06/26/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Smith, Jason R
Permit Number: 0024-7428
Effective:
09/29/2020-09/29/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	9:32pm
AIR BLK	.00	9:33pm
ACCY CHK	.07	9:34pm
AIR BLK	.00	9:34pm
SUB TEST	.00	9:35pm
AIR BLK	.00	9:36pm
SUB TEST	.00	9:37pm
AIR BLK	.00	9:38pm

Reported AC: .00 g/210L

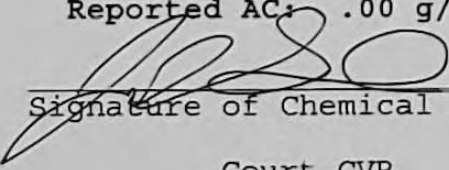

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 1 910

Serial Number: 008898 Test Record Number: 1165
Test Date: 06/26/2021 Test Time: 9:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:39pm
FLO	Pass	9:39pm
FC	Pass	9:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:40pm
SRC	Pass	9:40pm
DET	Pass	9:40pm
BAR	Pass	9:40pm
BT	Pass	9:40pm

Blank Tests

Test	Status	Time
AIR	Pass	9:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:40pm

CRC Tests

Test	Status	Time
COMP	Pass	9:41pm
CAL	Pass	9:41pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WASHINGTON Instrument Location SAF MARDE UNS 6

Instrument Serial No. 008584 PLYMOUTH

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of JUNE, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WASHINGTON COUNTY BAT MOBILE UNIT 6
930

Serial Number: 008584
Test Date: 06/05/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Varnell, Bryon L
Permit Number: 0036-1210
Effective:
08/14/2019-08/14/2021

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	10:58am
AIR BLK	.00	10:59am
ACCY CHK	.07	10:59am
AIR BLK	.00	11:00am
SUB TEST	.00	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:03am
AIR BLK	.00	11:04am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WASHINGTON COUNTY BAT MOBILE UNIT 6 930

Serial Number: 008584 Test Record Number: 2364
Test Date: 06/05/2021 Test Time: 11:07am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07am
FLO	Pass	11:07am
FC	Pass	11:07am

Temperature Tests

Test	Status	Time
FC1	Pass	11:08am
SRC	Pass	11:08am
DET	Pass	11:08am
BAR	Pass	11:08am
BT	Pass	11:08am

Blank Tests

Test	Status	Time
AIR	Pass	11:08am


Printer Tests

Test	Status	Time
PRNT	Pass	11:08am

CRC Tests

Test	Status	Time
COMP	Pass	11:08am
CAL	Pass	11:08am

Preventive Maintenance
Status: Pass

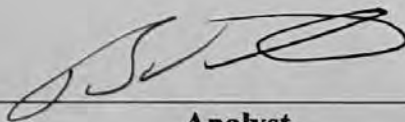

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Watauga Instrument Location Watauga Co. Jail
Instrument Serial No. 008715 Boone, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

049
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715
Test Date: 06/17/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401


Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	2:30pm
AIR BLK	.00	2:31pm
ACCY CHK	.08	2:31pm
AIR BLK	.00	2:32pm
SUB TEST	.00	2:33pm
AIR BLK	.00	2:34pm
SUB TEST	.00	2:35pm
AIR BLK	.00	2:36pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715 Test Record Number: 2530
Test Date: 06/17/2021 Test Time: 2:37pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:37pm
FLO	Pass	2:37pm
FC	Pass	2:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:37pm
SRC	Pass	2:37pm
DET	Pass	2:37pm
BAR	Pass	2:37pm
BT	Pass	2:37pm

Blank Tests

Test	Status	Time
AIR	Pass	2:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:38pm

CRC Tests

Test	Status	Time
COMP	Pass	2:38pm
CAL	Pass	2:38pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilson Instrument Location BAT Mobile Unit 4
Instrument Serial No. 008725 NL SHP

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY BAT MOBILE UNIT 4 970

Serial Number: 008775
Test Date: 06/05/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Smith, Jason R

Permit Number: 0024-7428

Effective:

09/29/2020-09/29/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	7:59pm
AIR BLK	.00	8:00pm
ACCY CHK	.07	8:01pm
AIR BLK	.00	8:02pm
SUB TEST	.00	8:02pm
AIR BLK	.00	8:03pm
SUB TEST	.00	8:05pm
AIR BLK	.00	8:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY BAT MOBILE UNIT 4 970

Serial Number: 008775 Test Record Number: 1870
Test Date: 06/05/2021 Test Time: 8:07pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:07pm
FLO	Pass	8:07pm
FC	Pass	8:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:07pm
SRC	Pass	8:07pm
DET	Pass	8:07pm
BAR	Pass	8:07pm
BT	Pass	8:07pm

Blank Tests

Test	Status	Time
AIR	Pass	8:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:08pm

CRC Tests

Test	Status	Time
COMP	Pass	8:08pm
CAL	Pass	8:08pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Yadkin Instrument Location Yadkin Co. Jail

Instrument Serial No. 009854 Yadkinville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: 008854
Test Date: 06/25/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:01pm
AIR BLK	.00	1:02pm
ACCY CHK	.08	1:02pm
AIR BLK	.00	1:03pm
SUB TEST	.00	1:04pm
AIR BLK	.00	1:05pm
SUB TEST	.00	1:06pm
AIR BLK	.00	1:07pm

Reported AC: .00 g/210L

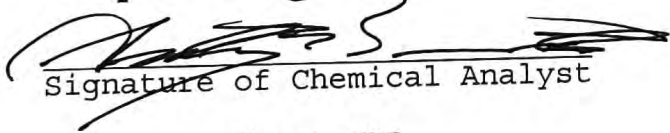
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: 008854 Test Record Number: 746
Test Date: 06/25/2021 Test Time: 1:08pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:09pm
FLO	Pass	1:09pm
FC	Pass	1:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:09pm
SRC	Pass	1:09pm
DET	Pass	1:09pm
BAR	Pass	1:09pm
BT	Pass	1:09pm

Blank Tests

Test	Status	Time
AIR	Pass	1:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:09pm

CRC Tests

Test	Status	Time
COMP	Pass	1:10pm
CAL	Pass	1:10pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Yadkin Instrument Location Yadkin Co. Jail
Instrument Serial No. 008944 Yadkinville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

644
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years

Intox EC/IR-II: Subject Test

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: 008944
Test Date: 06/25/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:01pm
AIR BLK	.00	1:02pm
ACCY CHK	.08	1:03pm
AIR BLK	.00	1:04pm
SUB TEST	.00	1:04pm
AIR BLK	.00	1:05pm
SUB TEST	.00	1:07pm
AIR BLK	.00	1:08pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: 008944 Test Record Number: 1696
Test Date: 06/25/2021 Test Time: 1:09pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:09pm
FLO	Pass	1:09pm
FC	Pass	1:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:09pm
SRC	Pass	1:09pm
DET	Pass	1:09pm
BAR	Pass	1:09pm
BT	Pass	1:09pm

Blank Tests

Test	Status	Time
AIR	Pass	1:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:10pm

CRC Tests

Test	Status	Time
COMP	Pass	1:10pm
CAL	Pass	1:10pm

Preventive Maintenance
Status: Pass



Analyst