

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Wendover C. Jail
Instrument Serial No. 104553 104 S Model II
Brookly, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. B. Smith
Signature of Certifying Official

1671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008853

Test Date: 09/29/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:35pm
AIR BLK	.00	1:36pm
ACCY CHK	.07	1:37pm
AIR BLK	.00	1:38pm
SUB TEST	.00	1:38pm
AIR BLK	.00	1:39pm
SUB TEST	.00	1:41pm
AIR BLK	.00	1:42pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008853 Test Record Number: 3534
Test Date: 09/29/2021 Test Time: 1:43pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:43pm
FLO	Pass	1:43pm
FC	Pass	1:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:44pm
SRC	Pass	1:44pm
DET	Pass	1:44pm
BAR	Pass	1:44pm
BT	Pass	1:44pm

Blank Tests

Test	Status	Time
AIR	Pass	1:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:44pm

CRC Tests

Test	Status	Time
COMP	Pass	1:44pm
CAL	Pass	1:44pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alamance Instrument Location Alamance Co Jail
Instrument Serial No. 1008913 1008913
Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913

Test Date: 09/29/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:43pm
AIR BLK	.00	1:43pm
ACCY CHK	.07	1:44pm
AIR BLK	.00	1:45pm
SUB TEST	.00	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913 Test Record Number: 4422
Test Date: 09/29/2021 Test Time: 1:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:55pm
FLO	Pass	1:55pm
FC	Pass	1:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:56pm

CRC Tests

Test	Status	Time
COMP	Pass	1:56pm
CAL	Pass	1:56pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Bladen Instrument Location BAT mobile Unit #5
Instrument Serial No. 008647 White Lake PD.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY BAT MOBILE UNIT 5 080

Serial Number: 008647

Test Date: 09/11/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703


Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	10:45pm
AIR BLK	.00	10:46pm
ACCY CHK	.07	10:47pm
AIR BLK	.00	10:48pm
SUB TEST	.00	10:49pm
AIR BLK	.00	10:50pm
SUB TEST	.00	10:51pm
AIR BLK	.00	10:52pm

Reported AC: .00 g/210L

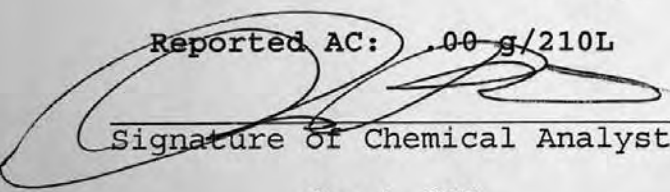
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY BAT MOBILE UNIT 5 080

Serial Number: 008647 Test Record Number: 2648

Test Date: 09/11/2021 Test Time: 10:53pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:54pm
FLO	Pass	10:54pm
FC	Pass	10:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:54pm
SRC	Pass	10:54pm
DET	Pass	10:54pm
BAR	Pass	10:54pm
BT	Pass	10:54pm

Blank Tests

Test	Status	Time
AIR	Pass	10:55pm

Printer Tests


Test	Status	Time
PRNT	Pass	10:55pm

CRC Tests

Test	Status	Time
COMP	Pass	10:55pm
CAL	Pass	10:55pm

Preventive Maintenance

Status: Pass

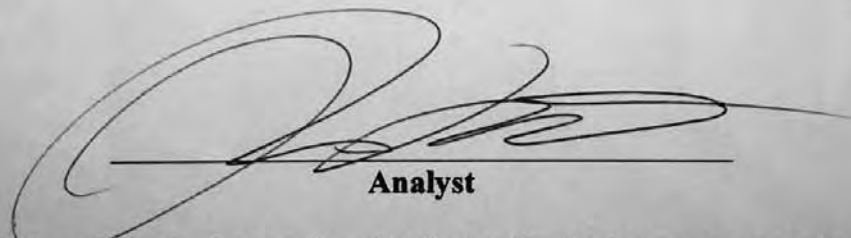

Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Bladen Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008826 White Lake P.D.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY BAT MOBILE UNIT 5 080

Serial Number: 008826
Test Date: 09/11/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG934303


Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	9:47pm
AIR BLK	.00	9:48pm
ACCY CHK	.08	9:48pm
AIR BLK	.00	9:49pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm
SUB TEST	.00	9:52pm
AIR BLK	.00	9:53pm

Reported AC: .00 g/210L

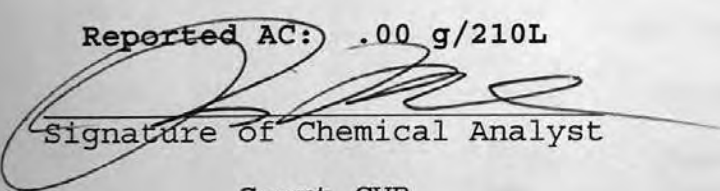
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY BAT MOBILE UNIT 5 080

Serial Number: 008826 Test Record Number: 8370
Test Date: 09/11/2021 Test Time: 9:55pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:55pm
FLO	Pass	9:55pm
FC	Pass	9:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:55pm
SRC	Pass	9:55pm
DET	Pass	9:55pm
BAR	Pass	9:55pm
BT	Pass	9:55pm

Blank Tests

Test	Status	Time
AIR	Pass	9:56pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:56pm

CRC Tests

Test	Status	Time
COMP	Pass	9:56pm
CAL	Pass	9:56pm

Preventive Maintenance
Status: Pass

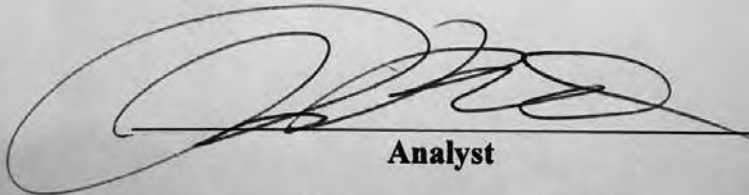

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Bladen Instrument Location Bladen County
Instrument Serial No. 008818 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of September, 2021 the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008818
Test Date: 09/27/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:44pm
AIR BLK	.00	1:44pm
ACCY CHK	.07	1:45pm
AIR BLK	.00	1:46pm
SUB TEST	.00	1:47pm
AIR BLK	.00	1:48pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm

Reported AC? .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008818 Test Record Number: 1859
Test Date: 09/27/2021 Test Time: 1:53pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:53pm
FLO	Pass	1:53pm
FC	Pass	1:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:54pm
SRC	Pass	1:54pm
DET	Pass	1:54pm
BAR	Pass	1:54pm
BT	Pass	1:54pm

Blank Tests

Test	Status	Time
AIR	Pass	1:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:54pm

CRC Tests

Test	Status	Time
COMP	Pass	1:54pm
CAL	Pass	1:54pm

Preventive Maintenance
Status: *Pass*

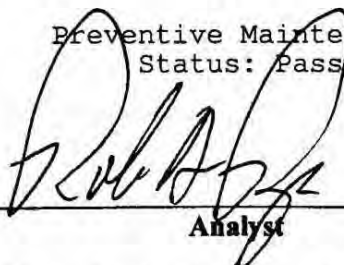

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Bladen Instrument Location Bladen County
Instrument Serial No. 008894 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of September, 2021, the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008894
Test Date: 09/27/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:45pm
AIR BLK	.00	1:46pm
ACCY CHK	.08	1:46pm
AIR BLK	.00	1:48pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:51pm
AIR BLK	.00	1:52pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008894 Test Record Number: 1317
Test Date: 09/27/2021 Test Time: 1:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:54pm
FLO	Pass	1:54pm
FC	Pass	1:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:54pm
SRC	Pass	1:54pm
DET	Pass	1:54pm
BAR	Pass	1:54pm
BT	Pass	1:54pm

Blank Tests

Test	Status	Time
AIR	Pass	1:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:55pm

CRC Tests

Test	Status	Time
COMP	Pass	1:55pm
CAL	Pass	1:55pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Brunswick Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008826 Brunswick County Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008826
Test Date: 09/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Todd, Shane C
Permit Number: 0035-4789
Effective:
10/06/2020-10/06/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG934303
Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	10:17pm
AIR BLK	.00	10:18pm
ACCY CHK	.08	10:19pm
AIR BLK	.00	10:20pm
SUB TEST	.00	10:21pm
AIR BLK	.00	10:21pm
SUB TEST	.00	10:23pm
AIR BLK	.00	10:24pm

Reported AC: .00 g/210L

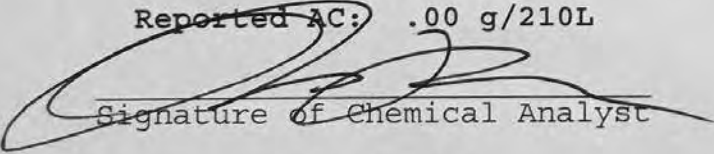
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008826 Test Record Number: 8365
Test Date: 09/03/2021 Test Time: 10:25pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:25pm
FLO	Pass	10:25pm
FC	Pass	10:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:26pm
SRC	Pass	10:26pm
DET	Pass	10:26pm
BAR	Pass	10:26pm
BT	Pass	10:26pm

Blank Tests

Test	Status	Time
AIR	Pass	10:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:26pm

CRC Tests

Test	Status	Time
COMP	Pass	10:26pm
CAL	Pass	10:26pm

Preventive Maintenance

Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Brunswick Instrument Location BAT Mobile Unit #5
Instrument Serial No. 608647 Brunswick County Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008647

Test Date: 09/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	10:21pm
AIR BLK	.00	10:22pm
ACCY CHK	.07	10:23pm
AIR BLK	.00	10:24pm
SUB TEST	.00	10:24pm
AIR BLK	.00	10:25pm
SUB TEST	.00	10:27pm
AIR BLK	.00	10:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090
Serial Number: 008647 Test Record Number: 2640
Test Date: 09/03/2021 Test Time: 10:30pm EDT
System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:30pm
FLO	Pass	10:30pm
FC	Pass	10:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:30pm
SRC	Pass	10:30pm
DET	Pass	10:30pm
BAR	Pass	10:30pm
BT	Pass	10:30pm

Blank Tests

Test	Status	Time
AIR	Pass	10:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:31pm

CRC Tests

Test	Status	Time
COMP	Pass	10:31pm
CAL	Pass	10:31pm

Preventive Maintenance
Status: Pass

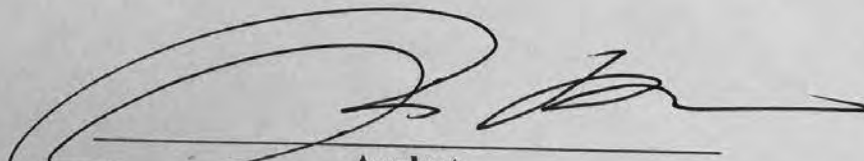

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location BAT Mobile Unit #9
Instrument Serial No. 008704 Brunswick County Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008704
Test Date: 09/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Todd, Shane C
Permit Number: 0035-4789
Effective:
10/06/2020-10/06/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG807101
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	10:19pm
AIR BLK	.00	10:20pm
ACCY CHK	.08	10:21pm
AIR BLK	.00	10:22pm
SUB TEST	.00	10:22pm
AIR BLK	.00	10:23pm
SUB TEST	.00	10:25pm
AIR BLK	.00	10:26pm

Reported AC: .00 g/210L

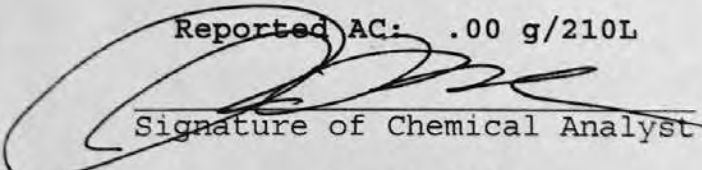
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008704 Test Record Number: 745
Test Date: 09/03/2021 Test Time: 10:27pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:27pm
FLO	Pass	10:27pm
FC	Pass	10:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:27pm
SRC	Pass	10:27pm
DET	Pass	10:27pm
BAR	Pass	10:27pm
BT	Pass	10:27pm

Blank Tests

Test	Status	Time
AIR	Pass	10:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:28pm

CRC Tests

Test	Status	Time
COMP	Pass	10:28pm
CAL	Pass	10:28pm

Preventive Maintenance
Status: Pass

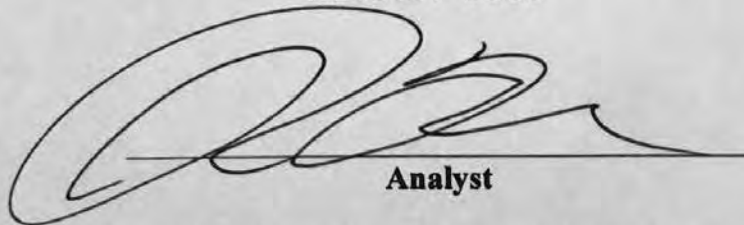

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Brunswick Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008826 Brunswick County Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008826
Test Date: 09/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Todd, Shane C
Permit Number: 0035-4789
Effective:
10/06/2020-10/06/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG934303
Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	10:17pm
AIR BLK	.00	10:18pm
ACCY CHK	.08	10:19pm
AIR BLK	.00	10:20pm
SUB TEST	.00	10:21pm
AIR BLK	.00	10:21pm
SUB TEST	.00	10:23pm
AIR BLK	.00	10:24pm

Reported AC: .00 g/210L

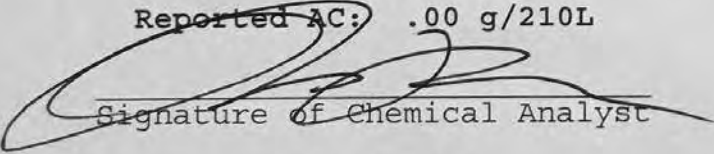
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008826 Test Record Number: 8365
Test Date: 09/03/2021 Test Time: 10:25pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:25pm
FLO	Pass	10:25pm
FC	Pass	10:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:26pm
SRC	Pass	10:26pm
DET	Pass	10:26pm
BAR	Pass	10:26pm
BT	Pass	10:26pm

Blank Tests

Test	Status	Time
AIR	Pass	10:26pm

Printer Tests


Test	Status	Time
PRNT	Pass	10:26pm

CRC Tests

Test	Status	Time
COMP	Pass	10:26pm
CAL	Pass	10:26pm

Preventive Maintenance

Status: Pass

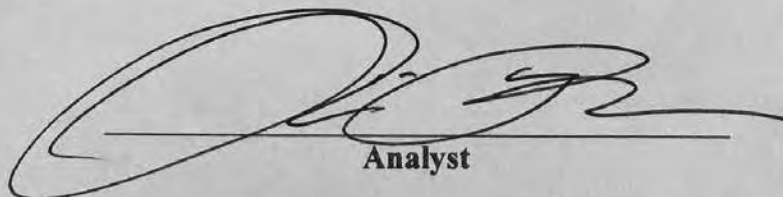

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location BAT Mobile Unit #9
Instrument Serial No. 008616 Brunswick County Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008616
Test Date: 09/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG933703


Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	4:54pm
AIR BLK	.00	4:55pm
ACCY GHK	.07	4:56pm
AIR BLK	.00	4:57pm
SUB TEST	.00	4:57pm
AIR BLK	.00	4:58pm
SUB TEST	.00	5:00pm
AIR BLK	.00	5:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

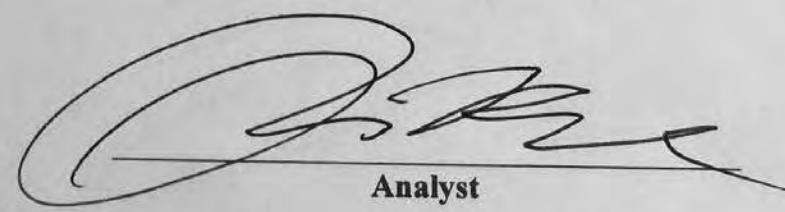
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008616 Test Record Number: 2649
Test Date: 09/03/2021 Test Time: 5:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:02pm
FLO	Pass	5:02pm
FC	Pass	5:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:02pm
SRC	Pass	5:02pm
DET	Pass	5:02pm
BAR	Pass	5:02pm
BT	Pass	5:02pm

Blank Tests

Test	Status	Time
AIR	Pass	5:03pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:03pm

CRC Tests

Test	Status	Time
COMP	Pass	5:03pm
CAL	Pass	5:03pm

Preventive Maintenance
Status: Pass

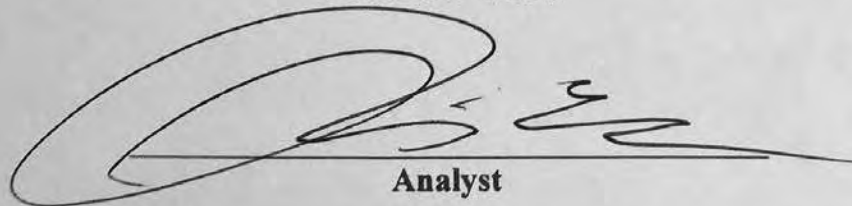

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location BAT Mobile Unit #9
Instrument Serial No. 008826 N.C.W.R.C

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008826

Test Date: 09/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG934303

Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	4:37pm
AIR BLK	.00	4:38pm
ACCY CHK	.07	4:39pm
AIR BLK	.00	4:40pm
SUB TEST	.00	4:40pm
AIR BLK	.00	4:41pm
SUB TEST	.00	4:43pm
AIR BLK	.00	4:44pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 5 090

Serial Number: 008826 Test Record Number: 8363
Test Date: 09/03/2021 Test Time: 4:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:45pm
FLO	Pass	4:45pm
FC	Pass	4:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:45pm
SRC	Pass	4:45pm
DET	Pass	4:45pm
BAR	Pass	4:45pm
BT	Pass	4:45pm

Blank Tests

Test	Status	Time
AIR	Pass	4:46pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:46pm

CRC Tests

Test	Status	Time
COMP	Pass	4:46pm
CAL	Pass	4:46pm

Preventive Maintenance
Status: Pass

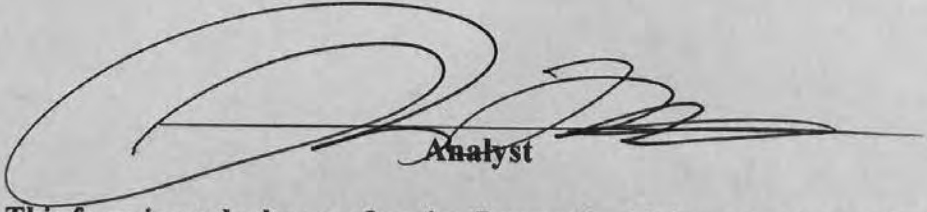

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location Black Mountain PD
Instrument Serial No. 006677 Black Mountain, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BLACK MOUNTAIN PD 100

Serial Number: 008697
Test Date: 09/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	4:59pm
AIR BLK	.00	4:59pm
ACCY CHK	.08	5:00pm
AIR BLK	.00	5:01pm
SUB TEST	.00	5:02pm
AIR BLK	.00	5:02pm
SUB TEST	.00	5:04pm
AIR BLK	.00	5:05pm

Reported AC: .00 g/210L

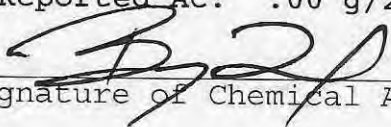
Signature of Chemical Analyst

Court CVR

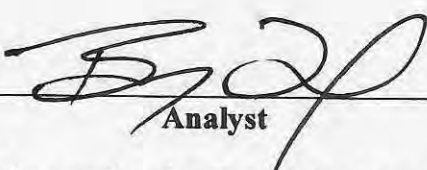
Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BLACK MOUNTAIN PD 100

Serial Number: 008697 Test Record Number: 3993
Test Date: 09/10/2021 Test Time: 5:05pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:05pm
FLO	Pass	5:05pm
FC	Pass	5:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:06pm
SRC	Pass	5:06pm
DET	Pass	5:06pm
BAR	Pass	5:06pm
BT	Pass	5:06pm

Blank Tests

Test	Status	Time
AIR	Pass	5:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:06pm

CRC Tests

Test	Status	Time
COMP	Pass	5:06pm
CAL	Pass	5:06pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caldwell Instrument Location Caldwell Co. Jail

Instrument Serial No. 008719 Lenoir, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6608
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008719
Test Date: 09/07/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:27am
AIR BLK	.00	10:28am
ACCY CHK	.07	10:29am
AIR BLK	.00	10:30am
SUB TEST	.00	10:31am
AIR BLK	.00	10:32am
SUB TEST	.00	10:33am
AIR BLK	.00	10:34am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008719 Test Record Number: 2886
Test Date: 09/07/2021 Test Time: 10:35am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:35am
FLO	Pass	10:35am
FC	Pass	10:35am

Temperature Tests

Test	Status	Time
FC1	Pass	10:35am
SRC	Pass	10:35am
DET	Pass	10:35am
BAR	Pass	10:35am
BT	Pass	10:35am

Blank Tests

Test	Status	Time
AIR	Pass	10:36am

Printer Tests

Test	Status	Time
PRNT	Pass	10:36am

CRC Tests

Test	Status	Time
COMP	Pass	10:36am
CAL	Pass	10:36am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Caldwell Instrument Location Caldwell Co Jail

Instrument Serial No. 009903 Lenoir, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

068
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008803
Test Date: 09/07/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	10:26am
AIR BLK	.00	10:27am
ACCY CHK	.07	10:28am
AIR BLK	.00	10:29am
SUB TEST	.00	10:30am
AIR BLK	.00	10:31am
SUB TEST	.00	10:32am
AIR BLK	.00	10:33am

Reported AC: .00 g/210L

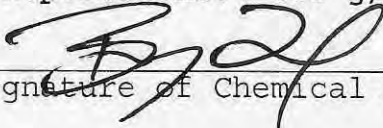

Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008803 Test Record Number: 750
Test Date: 09/07/2021 Test Time: 10:34am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:34am
FLO	Pass	10:34am
FC	Pass	10:34am

Temperature Tests

Test	Status	Time
FC1	Pass	10:34am
SRC	Pass	10:34am
DET	Pass	10:34am
BAR	Pass	10:34am
BT	Pass	10:34am

Blank Tests

Test	Status	Time
AIR	Pass	10:35am

Printer Tests

Test	Status	Time
PRNT	Pass	10:35am

CRC Tests

Test	Status	Time
COMP	Pass	10:35am
CAL	Pass	10:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CARTERET Instrument Location CARTERET COUNTY

Instrument Serial No. 008605 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Celen R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008605
Test Date: 09/27/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	4:25pm
AIR BLK	.00	4:26pm
ACCY CHK	.08	4:26pm
AIR BLK	.00	4:27pm
SUB TEST	.00	4:28pm
AIR BLK	.00	4:29pm
SUB TEST	.00	4:30pm
AIR BLK	.00	4:31pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008605 Test Record Number: 4082
Test Date: 09/27/2021 Test Time: 4:31pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:32pm
FLO	Pass	4:32pm
FC	Pass	4:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:32pm
SRC	Pass	4:32pm
DET	Pass	4:32pm
BAR	Pass	4:32pm
BT	Pass	4:32pm

Blank Tests

Test	Status	Time
AIR	Pass	4:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:33pm

CRC Tests

Test	Status	Time
COMP	Pass	4:33pm
CAL	Pass	4:33pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CARTERET Instrument Location EMERALD ISLE
Instrument Serial No. 008620 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008620

Test Date: 09/27/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	7:06pm
AIR BLK	.00	7:07pm
ACCY CHK	.08	7:08pm
AIR BLK	.00	7:09pm
SUB TEST	.00	7:09pm
AIR BLK	.00	7:10pm
SUB TEST	.00	7:12pm
AIR BLK	.00	7:13pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008620 Test Record Number: 2261
Test Date: 09/27/2021 Test Time: 7:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:13pm
FLO	Pass	7:13pm
FC	Pass	7:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:14pm
SRC	Pass	7:14pm
DET	Pass	7:14pm
BAR	Pass	7:14pm
BT	Pass	7:14pm

Blank Tests

Test	Status	Time
AIR	Pass	7:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:14pm

CRC Tests

Test	Status	Time
COMP	Pass	7:14pm
CAL	Pass	7:14pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CARTERET Instrument Location MOREHEAD CITY
Instrument Serial No. 008731 POLICE DEPT.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Basso
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731
Test Date: 09/27/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	3:26pm
AIR BLK	.00	3:27pm
ACCY CHK	.08	3:27pm
AIR BLK	.00	3:28pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm
SUB TEST	.00	3:31pm
AIR BLK	.00	3:32pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731 Test Record Number: 2376
Test Date: 09/27/2021 Test Time: 3:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:33pm
FLO	Pass	3:33pm
FC	Pass	3:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:33pm
SRC	Pass	3:33pm
DET	Pass	3:33pm
BAR	Pass	3:33pm
BT	Pass	3:33pm

Blank Tests

Test	Status	Time
AIR	Pass	3:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:34pm

CRC Tests

Test	Status	Time
COMP	Pass	3:34pm
CAL	Pass	3:34pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CARTERET Instrument Location ATLANTIC BEACH
Instrument Serial No. 008785 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of SEPTEMBER, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Celan R. Basso

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: 008785
Test Date: 09/27/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	5:29pm
AIR BLK	.00	5:30pm
ACCY CHK	.08	5:31pm
AIR BLK	.00	5:32pm
SUB TEST	.00	5:32pm
AIR BLK	.00	5:33pm
SUB TEST	.00	5:35pm
AIR BLK	.00	5:36pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: 008785 Test Record Number: 1314
Test Date: 09/27/2021 Test Time: 5:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:37pm
FLO	Pass	5:37pm
FC	Pass	5:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:37pm
SRC	Pass	5:37pm
DET	Pass	5:37pm
BAR	Pass	5:37pm
BT	Pass	5:37pm

Blank Tests

Test	Status	Time
AIR	Pass	5:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:38pm

CRC Tests

Test	Status	Time
COMP	Pass	5:38pm
CAL	Pass	5:38pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CARTERET Instrument Location CARTERET COUNTY
Instrument Serial No. 008882 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Rg B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008882
Test Date: 09/27/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	4:22pm
AIR BLK	.00	4:23pm
ACCY CHK	.08	4:23pm
AIR BLK	.00	4:24pm
SUB TEST	.00	4:25pm
AIR BLK	.00	4:26pm
SUB TEST	.00	4:28pm
AIR BLK	.00	4:29pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008882 Test Record Number: 2209
Test Date: 09/27/2021 Test Time: 4:29pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:29pm
FLO	Pass	4:29pm
FC	Pass	4:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:30pm
SRC	Pass	4:30pm
DET	Pass	4:30pm
BAR	Pass	4:30pm
BT	Pass	4:30pm

Blank Tests

Test	Status	Time
AIR	Pass	4:30pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:30pm

CRC Tests

Test	Status	Time
COMP	Pass	4:30pm
CAL	Pass	4:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Catawba Instrument Location Catawba County SO
Instrument Serial No. 008687 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687
Test Date: 09/02/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	1:42pm
AIR BLK	.00	1:43pm
ACCY CHK	.08	1:43pm
AIR BLK	.00	1:45pm
SUB TEST	.00	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:49pm
AIR BLK	.00	1:49pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687 Test Record Number: 3305
Test Date: 09/02/2021 Test Time: 1:52pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:52pm
FLO	Pass	1:52pm
FC	Pass	1:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:52pm
SRC	Pass	1:52pm
DET	Pass	1:52pm
BAR	Pass	1:52pm
BT	Pass	1:52pm

Blank Tests

Test	Status	Time
AIR	Pass	1:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:53pm

CRC Tests

Test	Status	Time
COMP	Pass	1:53pm
CAL	Pass	1:53pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Catawba Instrument Location Catawba County SO
Instrument Serial No. 008821 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821

Test Date: 09/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:42pm
AIR BLK	.00	1:43pm
ACCY CHK	.08	1:44pm
AIR BLK	.00	1:45pm
SUB TEST	.00	1:47pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:49pm
AIR BLK	.00	1:50pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821 Test Record Number: 2212
Test Date: 09/02/2021 Test Time: 1:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:52pm
FLO	Pass	1:52pm
FC	Pass	1:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:52pm
SRC	Pass	1:52pm
DET	Pass	1:52pm
BAR	Pass	1:52pm
BT	Pass	1:52pm

Blank Tests

Test	Status	Time
AIR	Pass	1:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:53pm

CRC Tests

Test	Status	Time
COMP	Pass	1:53pm
CAL	Pass	1:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Catawba Instrument Location Hickory Police Dept.
Instrument Serial No. 008841 Hickory, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841

Test Date: 09/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	3:07pm
AIR BLK	.00	3:08pm
ACCY CHK	.08	3:09pm
AIR BLK	.00	3:10pm
SUB TEST	.00	3:11pm
AIR BLK	.00	3:12pm
SUB TEST	.00	3:13pm
AIR BLK	.00	3:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841 Test Record Number: 2161
Test Date: 09/02/2021 Test Time: 3:15pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:15pm
FLO	Pass	3:15pm
FC	Pass	3:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:15pm
SRC	Pass	3:15pm
DET	Pass	3:15pm
BAR	Pass	3:15pm
BT	Pass	3:15pm

Blank Tests

Test	Status	Time
AIR	Pass	3:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:16pm

CRC Tests

Test	Status	Time
COMP	Pass	3:16pm
CAL	Pass	3:16pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Chowan Instrument Location Chowan Co Public Safety Center
Instrument Serial No. 008895 305 Freemason St, Edenton, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kay D

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895

Test Date: 09/14/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	12:34pm
AIR BLK	.00	12:34pm
ACCY CHK	.07	12:35pm
AIR BLK	.00	12:36pm
SUB TEST	.00	12:36pm
AIR BLK	.00	12:37pm
SUB TEST	.00	12:39pm
AIR BLK	.00	12:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895 Test Record Number: 1056
Test Date: 09/14/2021 Test Time: 12:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:41pm
FLO	Pass	12:41pm
FC	Pass	12:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:41pm
SRC	Pass	12:41pm
DET	Pass	12:41pm
BAR	Pass	12:41pm
BT	Pass	12:41pm

Blank Tests

Test	Status	Time
AIR	Pass	12:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:42pm

CRC Tests

Test	Status	Time
COMP	Pass	12:42pm
CAL	Pass	12:42pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Clay Instrument Location Clay Co. Jail

Instrument Serial No. 009608 Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608
Test Date: 09/08/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:22pm
AIR BLK	.00	1:22pm
ACCY CHK	.08	1:23pm
AIR BLK	.00	1:24pm
SUB TEST	.00	1:25pm
AIR BLK	.00	1:26pm
SUB TEST	.00	1:27pm
AIR BLK	.00	1:28pm

Reported AC: .00 g/210L

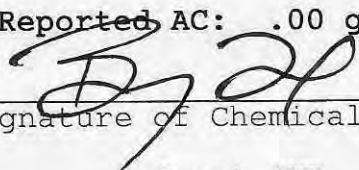

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608 Test Record Number: 1367
Test Date: 09/08/2021 Test Time: 1:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:29pm
FLO	Pass	1:29pm
FC	Pass	1:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:29pm
SRC	Pass	1:29pm
DET	Pass	1:29pm
BAR	Pass	1:29pm
BT	Pass	1:29pm

Blank Tests

Test	Status	Time
AIR	Pass	1:30pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:30pm

CRC Tests

Test	Status	Time
COMP	Pass	1:30pm
CAL	Pass	1:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cleveland Instrument Location Cleveland Co SO Annex
Instrument Serial No. 008893 Shelby, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Adams
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008893
Test Date: 09/08/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
04/20/2021-04/20/2023

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:39am
AIR BLK	.00	11:39am
ACCY CHK	.08	11:40am
AIR BLK	.00	11:41am
SUB TEST	.00	11:42am
AIR BLK	.00	11:42am
SUB TEST	.00	11:44am
AIR BLK	.00	11:45am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

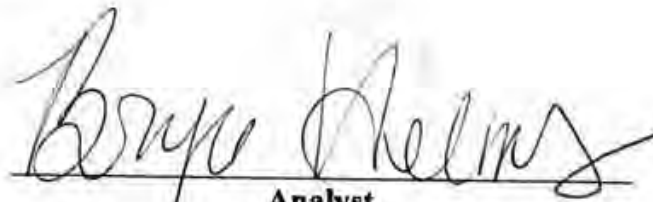
Analyst

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008893 Test Record Number: 1814
Test Date: 09/08/2021 Test Time: 11:48am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:48am
FLO	Pass	11:48am
FC	Pass	11:48am

Temperature Tests

Test	Status	Time
FC1	Pass	11:49am
SRC	Pass	11:49am
DET	Pass	11:49am
BAR	Pass	11:49am
BT	Pass	11:49am

Blank Tests

Test	Status	Time
AIR	Pass	11:49am


Printer Tests

Test	Status	Time
PRNT	Pass	11:49am

CRC Tests

Test	Status	Time
COMP	Pass	11:49am
CAL	Pass	11:49am

Preventive Maintenance
Status: Pass

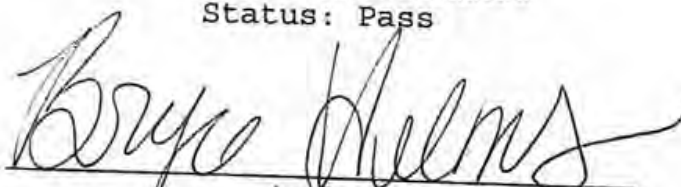

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cleveland Instrument Location Kings Mtn PD
Instrument Serial No. 008900 Kings Mtn, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900
Test Date: 09/08/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:37am
AIR BLK	.00	10:38am
ACCY CHK	.07	10:38am
AIR BLK	.00	10:39am
SUB TEST	.00	10:40am
AIR BLK	.00	10:41am
SUB TEST	.00	10:42am
AIR BLK	.00	10:43am

Reported AC: .00 g/210L

Bryce Helms

Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900 Test Record Number: 871
Test Date: 09/08/2021 Test Time: 10:44am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:44am
FLO	Pass	10:44am
FC	Pass	10:44am

Temperature Tests

Test	Status	Time
FC1	Pass	10:44am
SRC	Pass	10:44am
DET	Pass	10:44am
BAR	Pass	10:44am
BT	Pass	10:44am

Blank Tests

Test	Status	Time
AIR	Pass	10:45am


Printer Tests

Test	Status	Time
PRNT	Pass	10:45am

CRC Tests

Test	Status	Time
COMP	Pass	10:45am
CAL	Pass	10:45am

Preventive Maintenance
Status: Pass

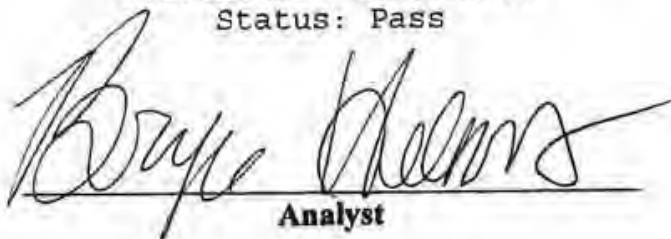
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cleveland Instrument Location Cleveland County SO- Annex
Instrument Serial No. 008910 Shelby, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boya Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO- ANNEX
220

Serial Number: 008910
Test Date: 09/09/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
04/20/2021-04/20/2023

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG035001
Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	1:49pm
AIR BLK	.00	1:49pm
ACCY CHK	.08	1:50pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:52pm
AIR BLK	.00	1:52pm
SUB TEST	.00	1:54pm
AIR BLK	.00	1:55pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO- ANNEX 220

Serial Number: 008910 Test Record Number: 1244
Test Date: 09/09/2021 Test Time: 1:56pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:56pm
FLO	Pass	1:56pm
FC	Pass	1:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:56pm
SRC	Pass	1:56pm
DET	Pass	1:56pm
BAR	Pass	1:56pm
BT	Pass	1:56pm

Blank Tests

Test	Status	Time
AIR	Pass	1:57pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:57pm

CRC Tests

Test	Status	Time
COMP	Pass	1:57pm
CAL	Pass	1:57pm

Preventive Maintenance
Status: Pass

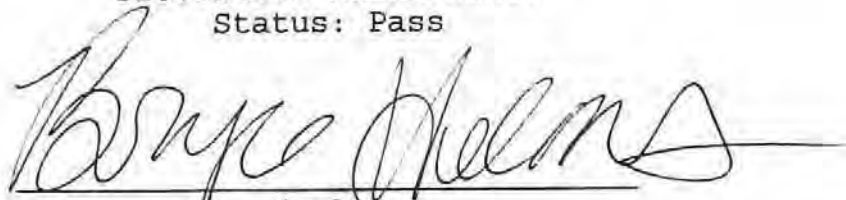

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Columbus Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008647 Columbus County Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus 2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008647

Test Date: 09/10/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	8:00pm
AIR BLK	.00	8:01pm
ACCY CHK	.07	8:02pm
AIR BLK	.00	8:02pm
SUB TEST	.00	8:03pm
AIR BLK	.00	8:04pm
SUB TEST	.00	8:06pm
AIR BLK	.00	8:07pm

Reported AC: .00 g/210L

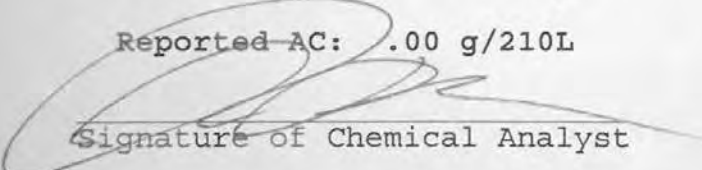
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 5 230
Serial Number: 008647 Test Record Number: 2644
Test Date: 09/10/2021 Test Time: 8:08pm EDT
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:09pm
FLO	Pass	8:09pm
FC	Pass	8:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:09pm
SRC	Pass	8:09pm
DET	Pass	8:09pm
BAR	Pass	8:09pm
BT	Pass	8:09pm

Blank Tests

Test	Status	Time
AIR	Pass	8:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:09pm

CRC Tests

Test	Status	Time
COMP	Pass	8:10pm
CAL	Pass	8:10pm

Preventive Maintenance
Status: Pass

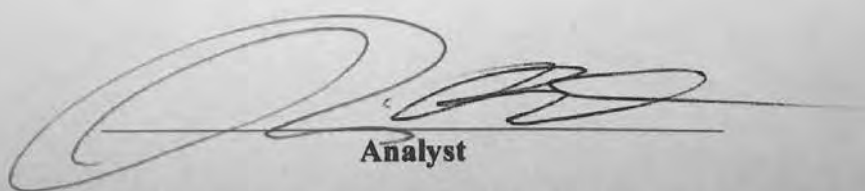

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Columbus Instrument Location Columbus County
Instrument Serial No. 008875 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008875
Test Date: 09/27/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	3:34pm
AIR BLK	.00	3:35pm
ACCY CHK	.07	3:35pm
AIR BLK	.00	3:36pm
SUB TEST	.00	3:37pm
AIR BLK	.00	3:38pm
SUB TEST	.00	3:39pm
AIR BLK	.00	3:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

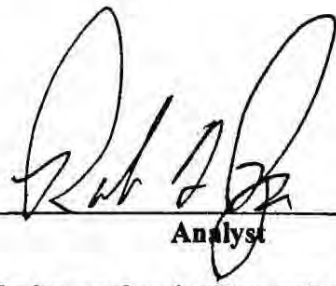

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008875 Test Record Number: 2528
Test Date: 09/27/2021 Test Time: 3:44pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:45pm
FLO	Pass	3:45pm
FC	Pass	3:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:45pm
SRC	Pass	3:45pm
DET	Pass	3:45pm
BAR	Pass	3:45pm
BT	Pass	3:45pm

Blank Tests

Test	Status	Time
AIR	Pass	3:46pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:46pm

CRC Tests

Test	Status	Time
COMP	Pass	3:46pm
CAL	Pass	3:46pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location Taber City
Instrument Serial No. 008886 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY TABOR CITY PD 230

Serial Number: 008886
Test Date: 09/28/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:15pm
AIR BLK	.00	1:15pm
ACCY CHK	.07	1:16pm
AIR BLK	.00	1:17pm
SUB TEST	.00	1:17pm
AIR BLK	.00	1:18pm
SUB TEST	.00	1:20pm
AIR BLK	.00	1:21pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY TABOR CITY PD 230

Serial Number: 008886 Test Record Number: 1597
Test Date: 09/28/2021 Test Time: 1:22pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:22pm
FLO	Pass	1:22pm
FC	Pass	1:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:22pm
SRC	Pass	1:22pm
DET	Pass	1:22pm
BAR	Pass	1:22pm
BT	Pass	1:22pm

Blank Tests

Test	Status	Time
AIR	Pass	1:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:23pm

CRC Tests

Test	Status	Time
COMP	Pass	1:23pm
CAL	Pass	1:23pm

Preventive Maintenance
Status: Pass

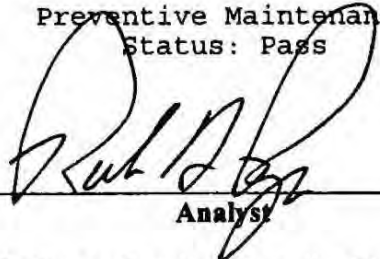

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Craven Instrument Location Havelock

Instrument Serial No. 008800 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY HAVELOCK PD 240

Serial Number: 008800
Test Date: 09/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023


Test	g/210L	Time
DIAG	Pass	11:17am
AIF: BLK	.00	11:17am
ACCY CHK	.07	11:18am
AIF: BLK	.00	11:19am
SUB: TEST	.00	11:19am
AIF: BLK	.00	11:20am
SUB: TEST	.00	11:22am
AIF: BLK	.00	11:23am

Reported AC: .00 g/210L

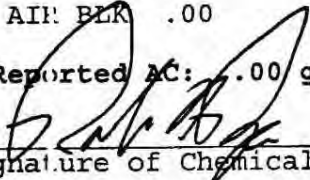

Signature of Chemical Analyst

Court CVR

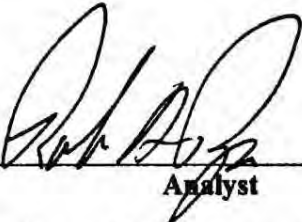

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY HAVELOCK PD 240

Serial Number: 008800 Test Record Number: 1429
Test Date: 09/02/2021 Test Time: 11:23am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:24am
FLO	Pass	11:24am
FC	Pass	11:24am

Temperature Tests

Test	Status	Time
FC1	Pass	11:24am
SRC	Pass	11:24am
DET	Pass	11:24am
BAR	Pass	11:24am
BT	Pass	11:24am

Blank Tests

Test	Status	Time
AIR	Pass	11:24am

Printer Tests


Test	Status	Time
PRNT	Pass	11:24am

CRC Tests

Test	Status	Time
COMP	Pass	11:25am
CAL	Pass	11:25am

Preventive Maintenance

Status: Pass

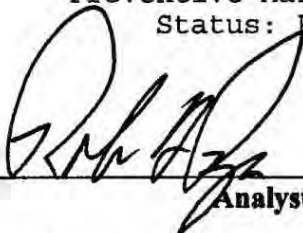

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CRAVEN Instrument Location CRAVEN COUNTY

Instrument Serial No. 008732 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY DETENTION CENTER 240

Serial Number: 008732
Test Date: 09/08/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107401

Exp Date: 03/15/2023


Test	g/210L	Time
DIAG	Pass	10:19am
AIR BLK	.00	10:19am
ACCY CHK	.07	10:20am
AIR BLK	.00	10:21am
SUB TEST	.00	10:22am
AIR BLK	.00	10:22am
SUB TEST	.00	10:24am
AIR BLK	.00	10:25am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY DETENTION CENTER 240

Serial Number: 008732 Test Record Number: 2650
Test Date: 09/08/2021 Test Time: 10:25am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:25am
FLO	Pass	10:25am
FC	Pass	10:26am

Temperature Tests

Test	Status	Time
FC1	Pass	10:26am
SRC	Pass	10:26am
DET	Pass	10:26am
BAR	Pass	10:26am
BT	Pass	10:26am

Blank Tests

Test	Status	Time
AIR	Pass	10:26am

Printer Tests

Test	Status	Time
PRNT	Pass	10:26am

CRC Tests

Test	Status	Time
COMP	Pass	10:27am
CAL	Pass	10:27am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CRAVEN Instrument Location NEW BERN

Instrument Serial No. 008817 POLICE DEPT.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Cheryl R. Benson
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY NEW BERN PD 240

Serial Number: 008817
Test Date: 09/08/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	11:46am
AIR BLK	.00	11:46am
ACCY CHK	.08	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:48am
AIR BLK	.00	11:49am
SUB TEST	.00	11:51am
AIR BLK	.00	11:51am

Reported AC: .00 g/210L

Alvin R. Barnes
Signature of Chemical Analyst

Court CVR

Alvin R. Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY NEW BERN PD 240

Serial Number: 008817 Test Record Number: 1688
Test Date: 09/08/2021 Test Time: 11:52am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:52am
FLO	Pass	11:52am
FC	Pass	11:52am

Temperature Tests

Test	Status	Time
FC1	Pass	11:52am
SRC	Pass	11:52am
DET	Pass	11:52am
BAR	Pass	11:52am
BT	Pass	11:52am

Blank Tests

Test	Status	Time
AIR	Pass	11:53am

Printer Tests

Test	Status	Time
PRNT	Pass	11:53am

CRC Tests

Test	Status	Time
COMP	Pass	11:53am
CAL	Pass	11:53am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location MCAS
Instrument Serial No. 010819 Cherry Point

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: 010819
Test Date: 09/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034901

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:10pm
AIR BLK	.00	1:11pm
ACCY CHK	.07	1:12pm
AIR BLK	.00	1:13pm
SUB TEST	.00	1:13pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:16pm
AIR BLK	.00	1:17pm

Reported AC: .00 g/210L

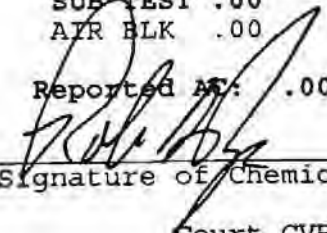

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: 010819 Test Record Number: 690
Test Date: 09/02/2021 Test Time: 1:18pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:18pm
FLO	Pass	1:18pm
FC	Pass	1:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:19pm
SRC	Pass	1:19pm
DET	Pass	1:19pm
BAR	Pass	1:19pm
BT	Pass	1:19pm

Blank Tests

Test	Status	Time
AIR	Pass	1:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:19pm

CRC Tests

Test	Status	Time
COMP	Pass	1:20pm
CAL	Pass	1:20pm

Preventive Maintenance
Status: *Pass*

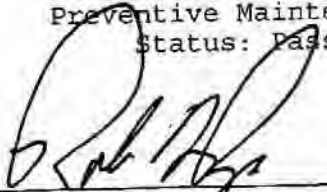

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location Kill Devil Hills P.D.

Instrument Serial No. 008844 107 Town Hall Dr., Kill Devil Hills NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kerr

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844
Test Date: 09/16/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	11:07am
AIR BLK	.00	11:08am
ACCY CHK	.07	11:08am
AIR BLK	.00	11:09am
SUB TEST	.00	11:10am
AIR BLK	.00	11:11am
SUB TEST	.00	11:12am
AIR BLK	.00	11:13am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844 Test Record Number: 2664
Test Date: 09/16/2021 Test Time: 11:14am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:15am
FLO	Pass	11:15am
FC	Pass	11:15am

Temperature Tests

Test	Status	Time
FC1	Pass	11:15am
SRC	Pass	11:15am
DET	Pass	11:15am
BAR	Pass	11:15am
BT	Pass	11:15am

Blank Tests

Test	Status	Time
AIR	Pass	11:15am

Printer Tests

Test	Status	Time
PRNT	Pass	11:15am

CRC Tests

Test	Status	Time
COMP	Pass	11:16am
CAL	Pass	11:16am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIDSON Instrument Location THOMASVILLE POLICE
Instrument Serial No. 008872 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1ST day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 669 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: 008872

Test Date: 09/01/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107502

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	3:34pm
AIR BLK	.00	3:35pm
ACCY CHK	.08	3:36pm
AIR BLK	.00	3:37pm
SUB TEST	.00	3:37pm
AIR BLK	.00	3:38pm
SUB TEST	.00	3:40pm
AIR BLK	.00	3:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: 008872 Test Record Number: 1556
Test Date: 09/01/2021 Test Time: 3:42pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:42pm
FLO	Pass	3:42pm
FC	Pass	3:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:42pm
SRC	Pass	3:42pm
DET	Pass	3:42pm
BAR	Pass	3:42pm
BT	Pass	3:42pm

Blank Tests

Test	Status	Time
AIR	Pass	3:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:43pm

CRC Tests

Test	Status	Time
COMP	Pass	3:43pm
CAL	Pass	3:43pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIE Instrument Location DAVIE COUNTY JAIL
Instrument Serial No. 008905 MOCKSVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3RD day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008905

Test Date: 09/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601


Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	4:43pm
AIR BLK	.00	4:44pm
ACCY CHK	.08	4:44pm
AIR BLK	.00	4:45pm
SUB TEST	.00	4:46pm
AIR BLK	.00	4:47pm
SUB TEST	.00	4:48pm
AIR BLK	.00	4:49pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

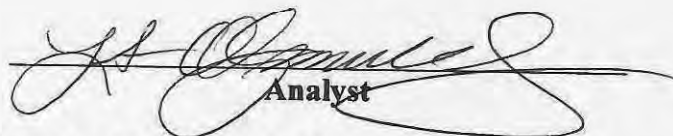
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008905 Test Record Number: 2603
Test Date: 09/03/2021 Test Time: 4:50pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:50pm
FLO	Pass	4:50pm
FC	Pass	4:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:50pm
SRC	Pass	4:50pm
DET	Pass	4:50pm
BAR	Pass	4:50pm
BT	Pass	4:50pm

Blank Tests

Test	Status	Time
AIR	Pass	4:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:51pm

CRC Tests

Test	Status	Time
COMP	Pass	4:51pm
CAL	Pass	4:51pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DUPLIN Instrument Location WALLACE

Instrument Serial No. 008858 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Celan Ry Bann
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008858
Test Date: 09/29/2021

Citation Number: M0000000-0

Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	3:48pm
AIR BLK	.00	3:48pm
ACCY CHK	.08	3:49pm
AIR BLK	.00	3:50pm
SUB TEST	.00	3:50pm
AIR BLK	.00	3:51pm
SUB TEST	.00	3:53pm
AIR BLK	.00	3:54pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008858 Test Record Number: 1112
Test Date: 09/29/2021 Test Time: 3:55pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:55pm
FLO	Pass	3:55pm
FC	Pass	3:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:55pm
SRC	Pass	3:55pm
DET	Pass	3:55pm
BAR	Pass	3:55pm
BT	Pass	3:55pm

Blank Tests

Test	Status	Time
AIR	Pass	3:56pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:56pm

CRC Tests

Test	Status	Time
COMP	Pass	3:56pm
CAL	Pass	3:56pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DUPLIN Instrument Location DUPLIN COUNTY
Instrument Serial No. 008864 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bana
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DUPLIN COUNTY DETENTION CENTER 300

Serial Number: 008864
Test Date: 09/29/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	5:25pm
AIR BLK	.00	5:26pm
ACCY CHK	.08	5:27pm
AIR BLK	.00	5:28pm
SUB TEST	.00	5:28pm
AIR BLK	.00	5:29pm
SUB TEST	.00	5:31pm
AIR BLK	.00	5:31pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY DETENTION CENTER 300

Serial Number: 008864 Test Record Number: 4218
Test Date: 09/29/2021 Test Time: 5:32pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:32pm
FLO	Pass	5:32pm
FC	Pass	5:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:32pm
SRC	Pass	5:32pm
DET	Pass	5:32pm
BAR	Pass	5:32pm
BT	Pass	5:32pm

Blank Tests

Test	Status	Time
AIR	Pass	5:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:33pm

CRC Tests

Test	Status	Time
COMP	Pass	5:33pm
CAL	Pass	5:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location FORSYTH COUNTY DETENTION
Instrument Serial No. 008583 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008583
Test Date: 09/29/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG118803

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	10:14am
AIR BLK	.00	10:15am
ACCY CHK	.08	10:16am
AIR BLK	.00	10:17am
SUB TEST	.00	10:18am
AIR BLK	.00	10:19am
SUB TEST	.00	10:21am
AIR BLK	.00	10:21am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008583 Test Record Number: 8571
Test Date: 09/29/2021 Test Time: 10:24am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:24am
FLO	Pass	10:24am
FC	Pass	10:24am

Temperature Tests

Test	Status	Time
FC1	Pass	10:24am
SRC	Pass	10:24am
DET	Pass	10:24am
BAR	Pass	10:24am
BT	Pass	10:24am

Blank Tests

Test	Status	Time
AIR	Pass	10:25am

Printer Tests

Test	Status	Time
PRNT	Pass	10:25am

CRC Tests

Test	Status	Time
COMP	Pass	10:25am
CAL	Pass	10:25am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location KERNERSVILLE POLICE

Instrument Serial No. 008650 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29TH day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650
Test Date: 09/29/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Oligmueller Jr., Leo A*
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933901
Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	11:08am
AIR BLK	.00	11:09am
ACCY CHK	.08	11:10am
AIR BLK	.00	11:11am
SUB TEST	.00	11:12am
AIR BLK	.00	11:13am
SUB TEST	.00	11:14am
AIR BLK	.00	11:15am

Reported AC: .00 g/210L

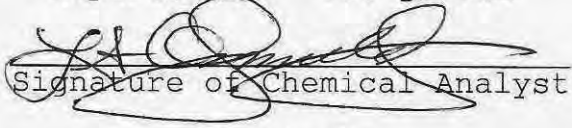
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650 Test Record Number: 1854
Test Date: 09/29/2021 Test Time: 11:16am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:16am
FLO	Pass	11:16am
FC	Pass	11:16am

Temperature Tests

Test	Status	Time
FC1	Pass	11:16am
SRC	Pass	11:16am
DET	Pass	11:16am
BAR	Pass	11:16am
BT	Pass	11:16am

Blank Tests

Test	Status	Time
AIR	Pass	11:17am

Printer Tests

Test	Status	Time
PRNT	Pass	11:17am

CRC Tests

Test	Status	Time
COMP	Pass	11:17am
CAL	Pass	11:17am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location FORSYTH CO. DETENTION

Instrument Serial No. 008660 WINSTON - SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21ST day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008660
Test Date: 09/21/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	1:05pm
AIR BLK	.00	1:07pm
ACCY CHK	.08	1:07pm
AIR BLK	.00	1:09pm
SUB TEST	.00	1:10pm
AIR BLK	.00	1:11pm
SUB TEST	.00	1:13pm
AIR BLK	.00	1:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008660 Test Record Number: 4397
Test Date: 09/21/2021 Test Time: 1:15pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:15pm
FLO	Pass	1:15pm
FC	Pass	1:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:15pm
SRC	Pass	1:15pm
DET	Pass	1:15pm
BAR	Pass	1:15pm
BT	Pass	1:15pm

Blank Tests

Test	Status	Time
AIR	Pass	1:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:16pm

CRC Tests

Test	Status	Time
COMP	Pass	1:16pm
CAL	Pass	1:16pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Franklin Instrument Location Franklin Co. LEC
Instrument Serial No. 008933 285 T. Kemp Rd
Louisburg, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008933

Test Date: 09/28/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	9:55am
AIR BLK	.00	9:55am
ACCY CHK	.07	9:56am
AIR BLK	.00	9:57am
SUB TEST	.00	9:58am
AIR BLK	.00	9:59am
SUB TEST	.00	10:00am
AIR BLK	.00	10:01am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008933 Test Record Number: 1291
Test Date: 09/28/2021 Test Time: 10:03am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:03am
FLO	Pass	10:03am
FC	Pass	10:03am

Temperature Tests

Test	Status	Time
FC1	Pass	10:03am
SRC	Pass	10:03am
DET	Pass	10:03am
BAR	Pass	10:03am
BT	Pass	10:03am

Blank Tests

Test	Status	Time
AIR	Pass	10:04am

Printer Tests

Test	Status	Time
PRNT	Pass	10:04am

CRC Tests

Test	Status	Time
COMP	Pass	10:04am
CAL	Pass	10:04am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Franklin Instrument Location Franklin Co. REC
Instrument Serial No. 008942 285 T Kemp Rd
Louisburg, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ed Smith Signature of Certifying Official 671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008942

Test Date: 09/28/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	9:56am
AIR BLK	.00	9:57am
ACCY CHK	.07	9:57am
AIR BLK	.00	9:59am
SUB TEST	.00	9:59am
AIR BLK	.00	10:00am
SUB TEST	.00	10:02am
AIR BLK	.00	10:03am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008942 Test Record Number: 2443
Test Date: 09/28/2021 Test Time: 10:04am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:04am
FLO	Pass	10:04am
FC	Pass	10:04am

Temperature Tests

Test	Status	Time
FC1	Pass	10:04am
SRC	Pass	10:04am
DET	Pass	10:04am
BAR	Pass	10:04am
BT	Pass	10:04am

Blank Tests

Test	Status	Time
AIR	Pass	10:05am

Printer Tests

Test	Status	Time
PRNT	Pass	10:05am

CRC Tests

Test	Status	Time
COMP	Pass	10:05am
CAL	Pass	10:05am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Mt. Holly PD
Instrument Serial No. 008733 Mt. Holly, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY MT. HOLLY PD 350

Serial Number: 008733

Test Date: 09/08/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001


Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	1:43pm
AIR BLK	.00	1:43pm
ACCY CHK	.07	1:44pm
AIR BLK	.00	1:45pm
SUB TEST	.00	1:46pm
AIR BLK	.00	1:46pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

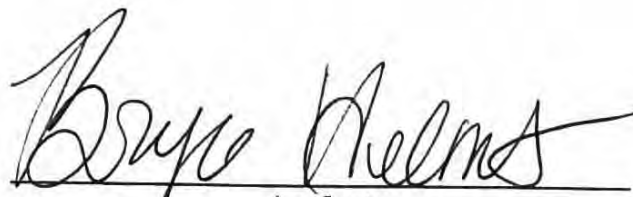
Analyst

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY MT. HOLLY PD 350

Serial Number: 008733 Test Record Number: 1275
Test Date: 09/08/2021 Test Time: 1:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:50pm
FLO	Pass	1:50pm
FC	Pass	1:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:50pm
SRC	Pass	1:50pm
DET	Pass	1:50pm
BAR	Pass	1:50pm
BT	Pass	1:50pm

Blank Tests

Test	Status	Time
AIR	Pass	1:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:51pm

CRC Tests

Test	Status	Time
COMP	Pass	1:51pm
CAL	Pass	1:51pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Craven Instrument Location BAT Mobile Unit 3
Instrument Serial No. 008971 Belmont PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY BAT MOBILE UNIT 3 350

Serial Number: 008971
Test Date: 09/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Smith, Jason R
Permit Number: 0024-7428
Effective:
09/29/2020-09/29/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	10:12pm
AIR BLK	.00	10:13pm
ACCY CHK	.07	10:14pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:15pm
AIR BLK	.00	10:16pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY BAT MOBILE UNIT 3 350

Serial Number: 008971 Test Record Number: 291
Test Date: 09/10/2021 Test Time: 10:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:22pm
FLO	Pass	10:22pm
FC	Pass	10:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:22pm
SRC	Pass	10:22pm
DET	Pass	10:22pm
BAR	Pass	10:22pm
BT	Pass	10:22pm

Blank Tests

Test	Status	Time
AIR	Pass	10:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:23pm

CRC Tests

Test	Status	Time
COMP	Pass	10:23pm
CAL	Pass	10:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Coaston Instrument Location BAT Mobile Unit 3
Instrument Serial No. 008972 Belmont PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY BAT MOBILE UNIT 3 350

Serial Number: 008972
Test Date: 09/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Smith, Jason R
Permit Number: 0024-7428
Effective:
09/29/2020-09/29/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:12pm
AIR BLK	.00	10:12pm
ACCY CHK	.07	10:13pm
AIR BLK	.00	10:14pm
SUB TEST	.00	10:14pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY BAT MOBILE UNIT 3 350

Serial Number: 008972 Test Record Number: 372
Test Date: 09/10/2021 Test Time: 10:20pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:20pm
FLO	Pass	10:20pm
FC	Pass	10:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:20pm
SRC	Pass	10:20pm
DET	Pass	10:20pm
BAR	Pass	10:20pm
BT	Pass	10:20pm

Blank Tests

Test	Status	Time
AIR	Pass	10:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:21pm

CRC Tests

Test	Status	Time
COMP	Pass	10:21pm
CAL	Pass	10:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Guilford Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008616 Gibsonville P.D.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 5 400

Serial Number: 008616 Test Record Number: 2656
Test Date: 09/24/2021 Test Time: 11:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:06pm
FLO	Pass	11:06pm
FC	Pass	11:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:06pm
SRC	Pass	11:06pm
DET	Pass	11:06pm
BAR	Pass	11:06pm
BT	Pass	11:06pm

Blank Tests

Test	Status	Time
AIR	Pass	11:07pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:07pm

CRC Tests

Test	Status	Time
COMP	Pass	11:07pm
CAL	Pass	11:07pm

Preventive Maintenance
Status: Pass

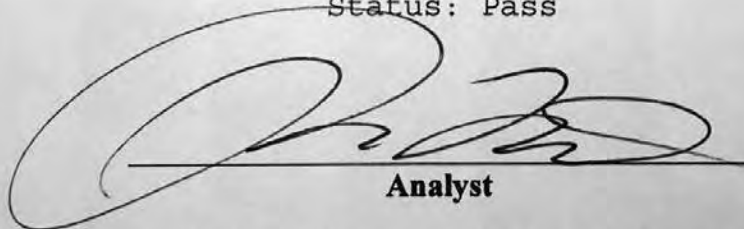

Analyst

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 5 400

Serial Number: 008616
Test Date: 09/24/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Todd, Shane C
Permit Number: 0035-4789
Effective:
10/06/2020-10/06/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933703
Exp Date: 12/03/2021


Test	g/210L	Time
DIAG	Pass	10:59pm
AIR BLK	.00	11:00pm
ACCY CHK	.07	11:00pm
AIR BLK	.00	11:01pm
SUB TEST	.00	11:02pm
AIR BLK	.00	11:02pm
SUB TEST	.00	11:04pm
AIR BLK	.00	11:05pm

Reported AC: .00 g/210L

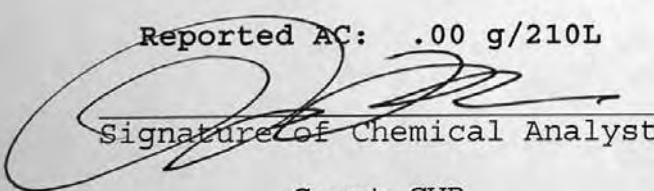

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Guilford Instrument Location BAT Mobile Unit #5
Instrument Serial No. 008826 Gibsonville P.D.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

664
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 5 400

Serial Number: 008826
Test Date: 09/24/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Todd, Shane C

Permit Number: 0035-4789

Effective:

10/06/2020-10/06/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG934303


Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	10:44pm
AIR BLK	.00	10:45pm
ACCY CHK	.07	10:46pm
AIR BLK	.00	10:46pm
SUB TEST	.00	10:47pm
AIR BLK	.00	10:48pm
SUB TEST	.00	10:50pm
AIR BLK	.00	10:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 5 400

Serial Number: 008826 Test Record Number: 8377
Test Date: 09/24/2021 Test Time: 10:52pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52pm
FLO	Pass	10:52pm
FC	Pass	10:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:52pm
SRC	Pass	10:52pm
DET	Pass	10:52pm
BAR	Pass	10:52pm
BT	Pass	10:52pm

Blank Tests

Test	Status	Time
AIR	Pass	10:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:53pm

CRC Tests

Test	Status	Time
COMP	Pass	10:53pm
CAL	Pass	10:53pm

Preventive Maintenance
Status: Pass

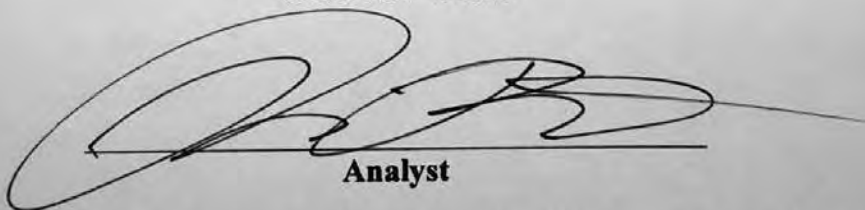

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County GUILFORD Instrument Location GREENSBORO JAIL

Instrument Serial No. 008790 GREENSBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13TH day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008790
Test Date: 09/13/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Oligmueller Jr., Leo A*
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	4:37pm
AIR BLK	.00	4:37pm
ACCY CHK	.08	4:38pm
AIR BLK	.00	4:39pm
SUB TEST	.00	4:39pm
AIR BLK	.00	4:40pm
SUB TEST	.00	4:42pm
AIR BLK	.00	4:43pm

Reported AC: .00 g/210L


Signature of Chemical Analyst
Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008790 Test Record Number: 7420
Test Date: 09/13/2021 Test Time: 4:43pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:44pm
FLO	Pass	4:44pm
FC	Pass	4:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:44pm
SRC	Pass	4:44pm
DET	Pass	4:44pm
BAR	Pass	4:44pm
BT	Pass	4:44pm

Blank Tests

Test	Status	Time
AIR	Pass	4:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:44pm

CRC Tests

Test	Status	Time
COMP	Pass	4:45pm
CAL	Pass	4:45pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hartford Instrument Location Abasco PD
Instrument Serial No. 008848 705 W. Main St, Abasco NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848
Test Date: 09/09/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Guard, Kelly G
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:27am
AIR BLK	.00	10:28am
ACCY CHK	.07	10:28am
AIR BLK	.00	10:29am
SUB TEST	.00	10:30am
AIR BLK	.00	10:31am
SUB TEST	.00	10:32am
AIR BLK	.00	10:33am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848 Test Record Number: 1626
Test Date: 09/09/2021 Test Time: 10:34am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:34am
FLO	Pass	10:34am
FC	Pass	10:35am

Temperature Tests

Test	Status	Time
FC1	Pass	10:35am
SRC	Pass	10:35am
DET	Pass	10:35am
BAR	Pass	10:35am
BT	Pass	10:35am

Blank Tests

Test	Status	Time
AIR	Pass	10:35am

Printer Tests

Test	Status	Time
PRNT	Pass	10:35am

CRC Tests

Test	Status	Time
COMP	Pass	10:35am
CAL	Pass	10:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hartford Instrument Location Murfreesboro P.D.

Instrument Serial No. 008906 115 E. Broad St., Murfreesboro, TN

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of September, 2011 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906
Test Date: 09/09/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Guard, Kelly G*
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:09pm
AIR BLK	.00	12:09pm
ACCY CHK	.08	12:10pm
AIR BLK	.00	12:11pm
SUB TEST	.00	12:12pm
AIR BLK	.00	12:13pm
SUB TEST	.00	12:14pm
AIR BLK	.00	12:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906 Test Record Number: 818
Test Date: 09/09/2021 Test Time: 12:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:18pm
FLO	Pass	12:18pm
FC	Pass	12:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:18pm
SRC	Pass	12:18pm
DET	Pass	12:18pm
BAR	Pass	12:18pm
BT	Pass	12:18pm

Blank Tests

Test	Status	Time
AIR	Pass	12:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:18pm

CRC Tests

Test	Status	Time
COMP	Pass	12:18pm
CAL	Pass	12:18pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hyde Instrument Location Hyde Co. S.O.

Instrument Serial No. 008861 1233 Main St, Sweet Quarter, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kel Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801
Test Date: 09/08/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021


Test	g/210L	Time
DIAG	Pass	10:42am
AIR BLK	.00	10:43am
ACCY CHK	.07	10:44am
AIR BLK	.00	10:45am
SUB TEST	.00	10:45am
AIR BLK	.00	10:46am
SUB TEST	.00	10:48am
AIR BLK	.00	10:48am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801 Test Record Number: 614
Test Date: 09/08/2021 Test Time: 10:49am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:50am
FLO	Pass	10:50am
FC	Pass	10:50am

Temperature Tests

Test	Status	Time
FC1	Pass	10:50am
SRC	Pass	10:50am
DET	Pass	10:50am
BAR	Pass	10:50am
BT	Pass	10:50am

Blank Tests

Test	Status	Time
AIR	Pass	10:51am

Printer Tests

Test	Status	Time
PRNT	Pass	10:51am

CRC Tests

Test	Status	Time
COMP	Pass	10:51am
CAL	Pass	10:51am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JOHNSTON Instrument Location SELMA POLICE
Instrument Serial No. 008595 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30TH day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595
Test Date: 09/30/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	4:05pm
AIR BLK	.00	4:06pm
ACCY CHK	.07	4:07pm
AIR BLK	.00	4:08pm
SUB TEST	.00	4:08pm
AIR BLK	.00	4:09pm
SUB TEST	.00	4:11pm
AIR BLK	.00	4:12pm

Reported AC: .00 g/210L

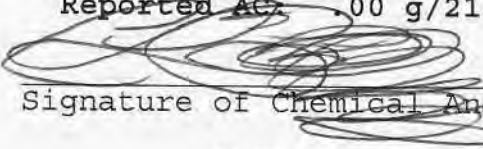
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595 Test Record Number: 1553
Test Date: 09/30/2021 Test Time: 4:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:14pm
FLO	Pass	4:14pm
FC	Pass	4:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:14pm
SRC	Pass	4:14pm
DET	Pass	4:14pm
BAR	Pass	4:14pm
BT	Pass	4:14pm

Blank Tests

Test	Status	Time
AIR	Pass	4:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:14pm

CRC Tests

Test	Status	Time
COMP	Pass	4:15pm
CAL	Pass	4:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JOHNSTON Instrument Location JOHNSTON COUNTY
Instrument Serial No. 008810 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30TH day of SEPTEMBER, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008810
Test Date: 09/30/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	2:20pm
AIR BLK	.00	2:20pm
ACCY CHK	.07	2:21pm
AIR BLK	.00	2:22pm
SUB TEST	.00	2:23pm
AIR BLK	.00	2:23pm
SUB TEST	.00	2:25pm
AIR BLK	.00	2:26pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008810 Test Record Number: 4665
Test Date: 09/30/2021 Test Time: 2:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:28pm
FLO	Pass	2:28pm
FC	Pass	2:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:28pm
SRC	Pass	2:28pm
DET	Pass	2:28pm
BAR	Pass	2:28pm
BT	Pass	2:28pm

Blank Tests

Test	Status	Time
AIR	Pass	2:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:29pm

CRC Tests

Test	Status	Time
COMP	Pass	2:29pm
CAL	Pass	2:29pm

Preventive Maintenance
Status: Pass

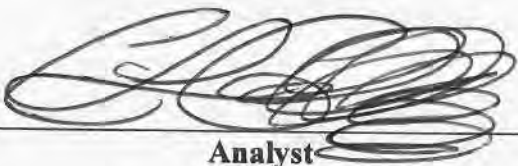

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JOHNSTON Instrument Location JOHNSTON COUNTY
Instrument Serial No. 008846 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30TH day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008846
Test Date: 09/30/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	2:21pm
AIR BLK	.00	2:22pm
ACCY CHK	.07	2:23pm
AIR BLK	.00	2:24pm
SUB TEST	.00	2:25pm
AIR BLK	.00	2:26pm
SUB TEST	.00	2:28pm
AIR BLK	.00	2:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008846 Test Record Number: 5563
Test Date: 09/30/2021 Test Time: 2:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:30pm
FLO	Pass	2:30pm
FC	Pass	2:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:30pm
SRC	Pass	2:30pm
DET	Pass	2:30pm
BAR	Pass	2:30pm
BT	Pass	2:30pm

Blank Tests

Test	Status	Time
AIR	Pass	2:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:31pm

CRC Tests

Test	Status	Time
COMP	Pass	2:31pm
CAL	Pass	2:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JOHNSTON Instrument Location BENSON POLICE
Instrument Serial No. 008885 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30TH day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BENSON PD 500

Serial Number: 008885
Test Date: 09/30/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034901


Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	12:29pm
AIR BLK	.00	12:30pm
ACCY CHK	.08	12:30pm
AIR BLK	.00	12:31pm
SUB TEST	.00	12:32pm
AIR BLK	.00	12:32pm
SUB TEST	.00	12:34pm
AIR BLK	.00	12:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BENSON PD 500

Serial Number: 008885 Test Record Number: 650
Test Date: 09/30/2021 Test Time: 12:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:37pm
FLO	Pass	12:37pm
FC	Pass	12:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:37pm
SRC	Pass	12:37pm
DET	Pass	12:37pm
BAR	Pass	12:37pm
BT	Pass	12:37pm

Blank Tests

Test	Status	Time
AIR	Pass	12:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:37pm

CRC Tests

Test	Status	Time
COMP	Pass	12:38pm
CAL	Pass	12:38pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Macon Instrument Location Macon Co Jail

Instrument Serial No. 008618 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008618
Test Date: 09/08/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	11:50am
AIR BLK	.00	11:50am
ACCY CHK	.07	11:51am
AIR BLK	.00	11:52am
SUB TEST	.00	11:53am
AIR BLK	.00	11:54am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008618 Test Record Number: 2197
Test Date: 09/08/2021 Test Time: 11:56am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:57am
FLO	Pass	11:57am
FC	Pass	11:57am

Temperature Tests

Test	Status	Time
FC1	Pass	11:57am
SRC	Pass	11:57am
DET	Pass	11:57am
BAR	Pass	11:57am
BT	Pass	11:57am

Blank Tests

Test	Status	Time
AIR	Pass	11:58am

Printer Tests

Test	Status	Time
PRNT	Pass	11:58am

CRC Tests

Test	Status	Time
COMP	Pass	11:58am
CAL	Pass	11:58am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Macon Instrument Location Macon Co. Jail

Instrument Serial No. 008789 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008789
Test Date: 09/08/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	11:49am
AIR BLK	.00	11:50am
ACCY CHK	.07	11:51am
AIR BLK	.00	11:52am
SUB TEST	.00	11:53am
AIR BLK	.00	11:54am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008789 Test Record Number: 735
Test Date: 09/08/2021 Test Time: 11:56am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:57am
FLO	Pass	11:57am
FC	Pass	11:57am

Temperature Tests

Test	Status	Time
FC1	Pass	11:57am
SRC	Pass	11:57am
DET	Pass	11:57am
BAR	Pass	11:57am
BT	Pass	11:57am

Blank Tests

Test	Status	Time
AIR	Pass	11:57am

Printer Tests

Test	Status	Time
PRNT	Pass	11:57am

CRC Tests

Test	Status	Time
COMP	Pass	11:58am
CAL	Pass	11:58am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Macon Instrument Location Macon Co Magistrate

Instrument Serial No. 008795 Highlands, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795

Test Date: 09/29/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	2:49pm
AIR BLK	.00	2:50pm
ACCY CHK	.08	2:50pm
AIR BLK	.00	2:51pm
SUB TEST	.00	2:52pm
AIR BLK	.00	2:53pm
SUB TEST	.00	2:54pm
AIR BLK	.00	2:55pm

Reported AC: .00 g/210L

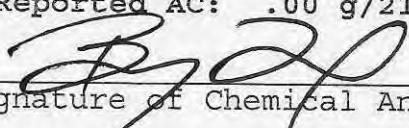

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795 Test Record Number: 546
Test Date: 09/29/2021 Test Time: 2:58pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:58pm
FLO	Pass	2:58pm
FC	Pass	2:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:58pm
SRC	Pass	2:58pm
DET	Pass	2:58pm
BAR	Pass	2:58pm
BT	Pass	2:58pm

Blank Tests

Test	Status	Time
AIR	Pass	2:59pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:59pm

CRC Tests

Test	Status	Time
COMP	Pass	2:59pm
CAL	Pass	2:59pm

Preventive Maintenance
Status: Pass

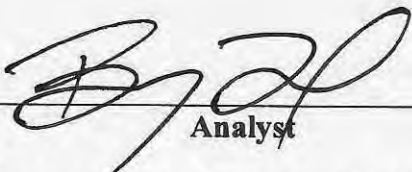

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Martin Instrument Location Martin Co. S.O.

Instrument Serial No. 008912 305 E. Main St., Williamston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912

Test Date: 09/14/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	2:31pm
AIR BLK	.00	2:32pm
ACCY CHK	.08	2:33pm
AIR BLK	.00	2:34pm
SUB TEST	.00	2:35pm
AIR BLK	.00	2:36pm
SUB TEST	.00	2:38pm
AIR BLK	.00	2:38pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912 Test Record Number: 1743
Test Date: 09/14/2021 Test Time: 2:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:46pm
FLO	Pass	2:46pm
FC	Pass	2:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:46pm
SRC	Pass	2:46pm
DET	Pass	2:46pm
BAR	Pass	2:46pm
BT	Pass	2:46pm

Blank Tests

Test	Status	Time
AIR	Pass	2:47pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:47pm

CRC Tests

Test	Status	Time
COMP	Pass	2:47pm
CAL	Pass	2:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County MECKLENBURG Instrument Location BAT MOBILE UNIT 6
Instrument Serial No. 008637 CHARLOTTE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of SEPTEMBER, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

663
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 6
590

Serial Number: 008637
Test Date: 09/16/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	10:06pm
AIR BLK	.00	10:07pm
ACCY CHK	.07	10:08pm
AIR BLK	.00	10:09pm
SUB TEST	.00	10:09pm
AIR BLK	.00	10:10pm
SUB TEST	.00	10:12pm
AIR BLK	.00	10:13pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 6 590

Serial Number: 008637 Test Record Number: 3152
Test Date: 09/16/2021 Test Time: 9:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:41pm
FLO	Pass	9:41pm
FC	Pass	9:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:41pm
SRC	Pass	9:41pm
DET	Pass	9:41pm
BAR	Pass	9:41pm
BT	Pass	9:41pm

Blank Tests

Test	Status	Time
AIR	Pass	9:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:42pm

CRC Tests

Test	Status	Time
COMP	Pass	9:42pm
CAL	Pass	9:42pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location BAT MOBILE UNIT 6
Instrument Serial No. 008776 CHARLOTTE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

663
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 6
590

Serial Number: 008776
Test Date: 09/15/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	8:08pm
AIR BLK	.00	8:09pm
ACCY CHK	.07	8:09pm
AIR BLK	.00	8:10pm
SUB TEST	.00	8:11pm
AIR BLK	.00	8:12pm
SUB TEST	.00	8:13pm
AIR BLK	.00	8:14pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

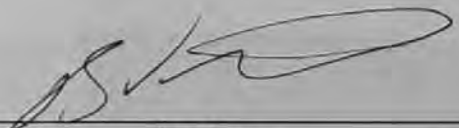

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 6 590

Serial Number: 008776 Test Record Number: 3680
Test Date: 09/15/2021 Test Time: 8:15pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:16pm
FLO	Pass	8:16pm
FC	Pass	8:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:16pm
SRC	Pass	8:16pm
DET	Pass	8:16pm
BAR	Pass	8:16pm
BT	Pass	8:16pm

Blank Tests

Test	Status	Time
AIR	Pass	8:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:16pm

CRC Tests

Test	Status	Time
COMP	Pass	8:17pm
CAL	Pass	8:17pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 6
Instrument Serial No. 008580 Nc WPC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 05 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 6
590

Serial Number: 008580
Test Date: 09/05/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Smith, Jason R

Permit Number: 0024-7428

Effective:

09/29/2020-09/29/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	4:04pm
AIR BLK	.00	4:05pm
ACCY CHK	.07	4:06pm
AIR BLK	.00	4:06pm
SUB TEST	.00	4:08pm
AIR BLK	.00	4:08pm
SUB TEST	.00	4:10pm
AIR BLK	.00	4:11pm

Reported AC: .00 g/210L

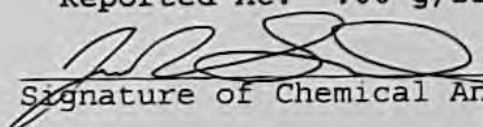
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 6 590

Serial Number: 008580 Test Record Number: 2637
Test Date: 09/05/2021 Test Time: 4:12pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:12pm
FLO	Pass	4:12pm
FC	Pass	4:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:12pm
SRC	Pass	4:12pm
DET	Pass	4:12pm
BAR	Pass	4:12pm
BT	Pass	4:12pm

Blank Tests

Test	Status	Time
AIR	Pass	4:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:13pm

CRC Tests

Test	Status	Time
COMP	Pass	4:13pm
CAL	Pass	4:13pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location CMPD LEC
Instrument Serial No. 0086911 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryan Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691
Test Date: 09/15/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804


Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	1:33pm
AIR BLK	.00	1:34pm
ACCY CHK	.08	1:34pm
AIR BLK	.00	1:35pm
SUB TEST	.00	1:36pm
AIR BLK	.00	1:37pm
SUB TEST	.00	1:38pm
AIR BLK	.00	1:39pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

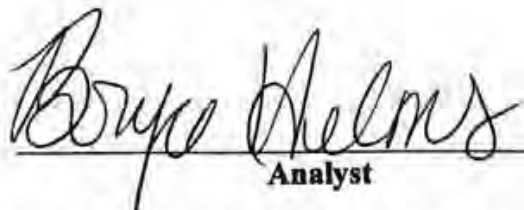
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691 Test Record Number: 8523
Test Date: 09/15/2021 Test Time: 1:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:42pm
FLO	Pass	1:42pm
FC	Pass	1:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:42pm
SRC	Pass	1:42pm
DET	Pass	1:42pm
BAR	Pass	1:42pm
BT	Pass	1:42pm

Blank Tests

Test	Status	Time
AIR	Pass	1:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:42pm

CRC Tests

Test	Status	Time
COMP	Pass	1:43pm
CAL	Pass	1:43pm

Preventive Maintenance
Status: Pass

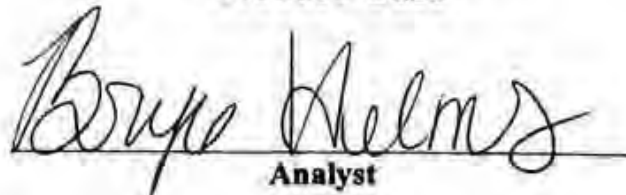
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Cornelius PD
Instrument Serial No. 008092 Cornelius, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692
Test Date: 09/07/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
04/20/2021-04/20/2023

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:46am
AIR BLK	.00	11:46am
ACCY CHK	.07	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:48am
AIR BLK	.00	11:49am
SUB TEST	.00	11:51am
AIR BLK	.00	11:52am

Reported AG: .00 g/210L


Signature of Chemical Analyst

Court CVR

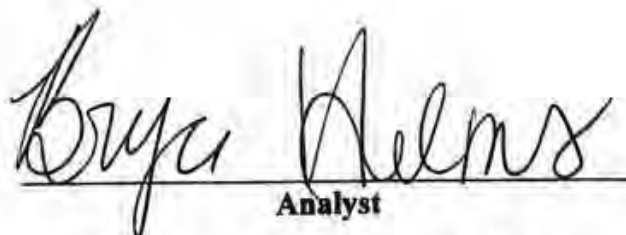
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692 Test Record Number: 3156
Test Date: 09/07/2021 Test Time: 11:53am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:53am
FLO	Pass	11:53am
FC	Pass	11:53am

Temperature Tests

Test	Status	Time
FC1	Pass	11:53am
SRC	Pass	11:53am
DET	Pass	11:53am
BAR	Pass	11:53am
BT	Pass	11:53am

Blank Tests

Test	Status	Time
AIR	Pass	11:54am


Printer Tests

Test	Status	Time
PRNT	Pass	11:54am

CRC Tests

Test	Status	Time
COMP	Pass	11:54am
CAL	Pass	11:54am

Preventive Maintenance
Status: *Pass*

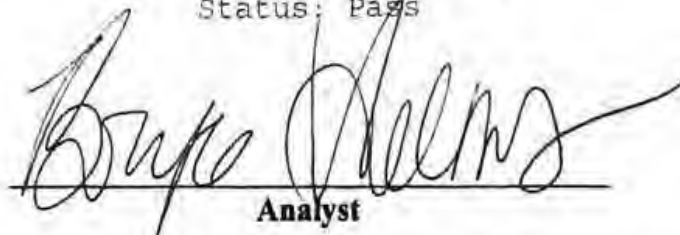
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mitchell Instrument Location Spencer Pine Police Dept
Instrument Serial No. 009726 Spencer Pine, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MITCHELL COUNTY SPRUCE PINE PD 600

Serial Number: 008726
Test Date: 09/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	10:47am
AIR BLK	.00	10:47am
ACCY CHK	.08	10:48am
AIR BLK	.00	10:49am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am

Reported AC: .00 g/210L

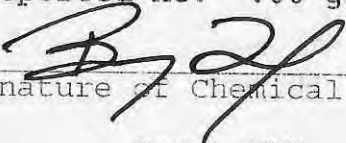
Signature of Chemical Analyst
Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MITCHELL COUNTY SPRUCE PINE PD 600

Serial Number: 008726 Test Record Number: 1148
Test Date: 09/02/2021 Test Time: 10:54am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:54am
FLO	Pass	10:54am
FC	Pass	10:54am

Temperature Tests

Test	Status	Time
FC1	Pass	10:54am
SRC	Pass	10:54am
DET	Pass	10:54am
BAR	Pass	10:54am
BT	Pass	10:54am

Blank Tests

Test	Status	Time
AIR	Pass	10:55am

Printer Tests

Test	Status	Time
PRNT	Pass	10:55am

CRC Tests

Test	Status	Time
COMP	Pass	10:55am
CAL	Pass	10:55am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH Instrument Location JAT MOBILE UNIT 6

Instrument Serial No. 008637 ROCKY MOUNT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008637

Test Date: 09/10/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	11:27pm
AIR BLK	.00	11:28pm
ACCY CHK	.07	11:28pm
AIR BLK	.00	11:29pm
SUB TEST	.00	11:30pm
AIR BLK	.00	11:31pm
SUB TEST	.00	11:32pm
AIR BLK	.00	11:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008637 Test Record Number: 3147
Test Date: 09/10/2021 Test Time: 11:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:35pm
FLO	Pass	11:35pm
FC	Pass	11:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:35pm
SRC	Pass	11:35pm
DET	Pass	11:35pm
BAR	Pass	11:35pm
BT	Pass	11:35pm

Blank Tests

Test	Status	Time
AIR	Pass	11:36pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:36pm

CRC Tests

Test	Status	Time
COMP	Pass	11:36pm
CAL	Pass	11:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NASH Instrument Location NAT MONIE UNIT 6

Instrument Serial No. 008776 ROCKY MOUNT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008776

Test Date: 09/10/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001


Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	11:28pm
AIR BLK	.00	11:29pm
ACCY CHK	.07	11:30pm
AIR BLK	.00	11:30pm
SUB TEST	.00	11:31pm
AIR BLK	.00	11:32pm
SUB TEST	.00	11:33pm
AIR BLK	.00	11:34pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008776 Test Record Number: 3674
Test Date: 09/10/2021 Test Time: 11:48pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:49pm
FLO	Pass	11:49pm
FC	Pass	11:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:49pm
SRC	Pass	11:49pm
DET	Pass	11:49pm
BAR	Pass	11:49pm
BT	Pass	11:49pm

Blank Tests

Test	Status	Time
AIR	Pass	11:49pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:49pm

CRC Tests

Test	Status	Time
COMP	Pass	11:50pm
CAL	Pass	11:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH Instrument Location BAT MONTIC UNIT 6
Instrument Serial No. 008179 POCKET MOUNT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus 2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

663

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008779
Test Date: 09/10/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	11:26pm
AIR BLK	.00	11:27pm
ACCY CHK	.07	11:27pm
AIR BLK	.00	11:28pm
SUB TEST	.00	11:29pm
AIR BLK	.00	11:30pm
SUB TEST	.00	11:31pm
AIR BLK	.00	11:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

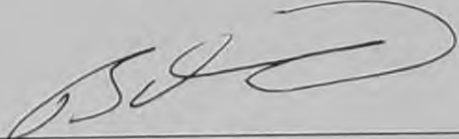

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008779 Test Record Number: 3718
Test Date: 09/10/2021 Test Time: 11:33pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:33pm
FLO	Pass	11:33pm
FC	Pass	11:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:33pm
SRC	Pass	11:33pm
DET	Pass	11:33pm
BAR	Pass	11:33pm
BT	Pass	11:33pm

Blank Tests

Test	Status	Time
AIR	Pass	11:34pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:34pm

CRC Tests

Test	Status	Time
COMP	Pass	11:34pm
CAL	Pass	11:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Nash Instrument Location Nash Co. Detention Ctr.
Instrument Serial No. U08630 222 S. Washington St
Nashville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ed Bruster
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY NASH DETENTION CTR 630

Serial Number: 008630

Test Date: 09/10/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501


Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	12:53pm
AIR BLK	.00	12:54pm
ACCY CHK	.08	12:54pm
AIR BLK	.00	12:55pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:57pm
SUB TEST	.00	12:58pm
AIR BLK	.00	12:59pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY NASH DETENTION CTR 630

Serial Number: 008630 Test Record Number: 5155
Test Date: 09/10/2021 Test Time: 1:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:00pm
FLO	Pass	1:00pm
FC	Pass	1:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:00pm
SRC	Pass	1:00pm
DET	Pass	1:00pm
BAR	Pass	1:00pm
BT	Pass	1:00pm

Blank Tests

Test	Status	Time
AIR	Pass	1:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:01pm

CRC Tests

Test	Status	Time
COMP	Pass	1:01pm
CAL	Pass	1:01pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location Rocky Mount PD
Instrument Serial No. 008740 #1 GOVERNMENT PLAZA
Rocky Mount, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008740

Test Date: 09/10/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	11:35am
AIR BLK	.00	11:36am
ACCY CHK	.07	11:36am
AIR BLK	.00	11:37am
SUB TEST	.00	11:38am
AIR BLK	.00	11:39am
SUB TEST	.00	11:40am
AIR BLK	.00	11:41am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008740 Test Record Number: 787
Test Date: 09/10/2021 Test Time: 11:42am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:43am
FLO	Pass	11:43am
FC	Pass	11:43am

Temperature Tests

Test	Status	Time
FC1	Pass	11:43am
SRC	Pass	11:43am
DET	Pass	11:43am
BAR	Pass	11:43am
BT	Pass	11:43am

Blank Tests

Test	Status	Time
AIR	Pass	11:43am

Printer Tests

Test	Status	Time
PRNT	Pass	11:43am

CRC Tests

Test	Status	Time
COMP	Pass	11:44am
CAL	Pass	11:44am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wash Instrument Location Rocky Mount PD
Instrument Serial No. 008741 41 Government Plaza
Rocky Mount, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008741

Test Date: 09/10/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	11:50am
AIR BLK	.00	11:51am
ACCY CHK	.07	11:51am
AIR BLK	.00	11:52am
SUB TEST	.00	11:53am
AIR BLK	.00	11:54am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008741 Test Record Number: 2819
Test Date: 09/10/2021 Test Time: 11:57am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:57am
FLO	Pass	11:57am
FC	Pass	11:57am

Temperature Tests

Test	Status	Time
FC1	Pass	11:57am
SRC	Pass	11:57am
DET	Pass	11:57am
BAR	Pass	11:57am
BT	Pass	11:57am

Blank Tests

Test	Status	Time
AIR	Pass	11:58am


Printer Tests

Test	Status	Time
PRNT	Pass	11:58am

CRC Tests

Test	Status	Time
COMP	Pass	11:58am
CAL	Pass	11:58am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County New Hanover Instrument Location New Hanover County
Instrument Serial No. 008617 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008617
Test Date: 09/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	3:53pm
AIR BLK	.00	3:54pm
ACCY CHK	.07	3:55pm
AIR BLK	.00	3:56pm
SUB TEST	.00	3:57pm
AIR BLK	.00	3:57pm
SUB TEST	.00	3:59pm
AIR BLK	.00	4:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008617 Test Record Number: 3731
Test Date: 09/03/2021 Test Time: 4:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:01pm
FLO	Pass	4:01pm
FC	Pass	4:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:02pm
SRC	Pass	4:02pm
DET	Pass	4:02pm
BAR	Pass	4:02pm
BT	Pass	4:02pm

Blank Tests

Test	Status	Time
AIR	Pass	4:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:02pm

CRC Tests

Test	Status	Time
COMP	Pass	4:02pm
CAL	Pass	4:02pm

Preventive Maintenance
Status: *Pass*

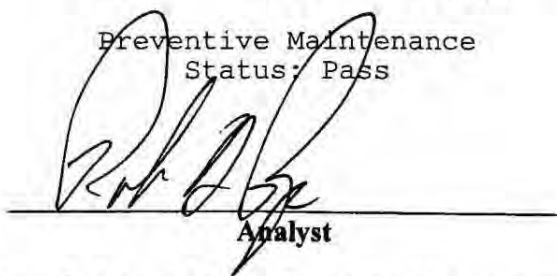

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County New Hanover Instrument Location New Hanover County

Instrument Serial No. 008626 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of September, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Handwritten signature of the certifying official.

Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008626
Test Date: 09/03/2021


Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	3:52pm
AIR BLK	.00	3:53pm
ACCY CHK	.08	3:54pm
AIR BLK	.00	3:55pm
SUB TEST	.00	3:55pm
AIR BLK	.00	3:56pm
SUB TEST	.00	3:58pm
AIR BLK	.00	3:59pm

Reported AC:  .00 g/210L

Signature of Chemical Analyst

Court CVR

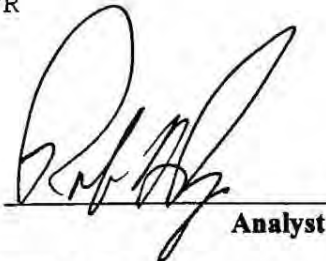

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008626 Test Record Number: 8022
Test Date: 09/03/2021 Test Time: 4:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:00pm
FLO	Pass	4:00pm
FC	Pass	4:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:00pm
SRC	Pass	4:00pm
DET	Pass	4:00pm
BAR	Pass	4:00pm
BT	Pass	4:00pm

Blank Tests

Test	Status	Time
AIR	Pass	4:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:01pm

CRC Tests

Test	Status	Time
COMP	Pass	4:01pm
CAL	Pass	4:01pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County New Hanover Instrument Location BAT mobile unit 1

Instrument Serial No. 008939 wilmington

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

New Hanover

~~ONSLOW~~ COUNTY BAT MOBILE UNIT 1 640

Serial Number: 008939

Test Date: 09/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	2:44pm
AIR BLK	.00	2:45pm
ACCY CHK	.08	2:45pm
AIR BLK	.00	2:46pm
SUB TEST	.00	2:47pm
AIR BLK	.00	2:48pm
SUB TEST	.00	2:49pm
AIR BLK	.00	2:50pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

New Hanover

ONSLOW COUNTY BAT MOBILE UNIT 1 640

Serial Number: 008939 Test Record Number: 1089
Test Date: 09/03/2021 Test Time: 2:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:52pm
SRC	Pass	2:52pm
DET	Pass	2:52pm
BAR	Pass	2:52pm
BT	Pass	2:52pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:53pm
CAL	Pass	2:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County onslow Instrument Location DAT Mobile Unit 7

Instrument Serial No. 008898 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 1 660

Serial Number: 008898
Test Date: 09/30/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	9:51pm
AIR BLK	.00	9:52pm
ACCY CHK	.07	9:53pm
AIR BLK	.00	9:54pm
SUB TEST	.00	9:54pm
AIR BLK	.00	9:55pm
SUB TEST	.00	9:57pm
AIR BLK	.00	9:58pm

Reported AC: ~~.00~~ g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 1 660

Serial Number: 008898 Test Record Number: 1209
Test Date: 09/30/2021 Test Time: 9:59pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:59pm
FLO	Pass	9:59pm
FC	Pass	9:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:59pm
SRC	Pass	9:59pm
DET	Pass	9:59pm
BAR	Pass	9:59pm
BT	Pass	9:59pm

Blank Tests

Test	Status	Time
AIR	Pass	10:00pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:00pm

CRC Tests

Test	Status	Time
COMP	Pass	10:00pm
CAL	Pass	10:00pm

Preventive Maintenance
Status: Pass

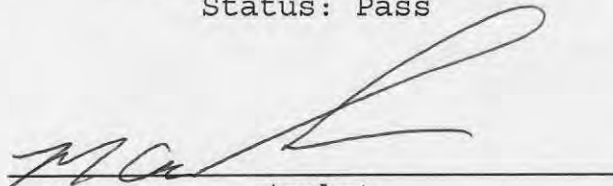

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT mobile unit I

Instrument Serial No. 008898 Jacksonville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mace
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 1 660

Serial Number: 008898
Test Date: 09/01/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	10:10pm
AIR BLK	.00	10:11pm
ACCY CHK	.07	10:11pm
AIR BLK	.00	10:12pm
SUB TEST	.00	10:13pm
AIR BLK	.00	10:14pm
SUB TEST	.00	10:15pm
AIR BLK	.00	10:16pm

Reported AC: .00 g/210L

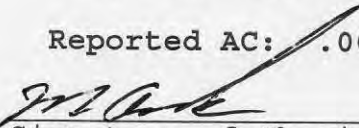

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 1 660

Serial Number: 008898 Test Record Number: 1188
Test Date: 09/01/2021 Test Time: 10:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:21pm
FLO	Pass	10:21pm
FC	Pass	10:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:21pm
SRC	Pass	10:21pm
DET	Pass	10:21pm
BAR	Pass	10:21pm
BT	Pass	10:21pm

Blank Tests

Test	Status	Time
AIR	Pass	10:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:22pm

CRC Tests

Test	Status	Time
COMP	Pass	10:22pm
CAL	Pass	10:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONslow Instrument Location MCAS NEW RIVER
Instrument Serial No. 008919 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bantz
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY MCAS NEW RIVER 660

Serial Number: 008919
Test Date: 09/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	2:27pm
AIR BLK	.00	2:27pm
ACCY CHK	.07	2:28pm
AIR BLK	.00	2:29pm
SUB TEST	.00	2:30pm
AIR BLK	.00	2:31pm
SUB TEST	.00	2:32pm
AIR BLK	.00	2:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLow COUNTY MCAS NEW RIVER 660

Serial Number: 008919 Test Record Number: 751
Test Date: 09/10/2021 Test Time: 2:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:35pm
FLO	Pass	2:35pm
FC	Pass	2:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:35pm
SRC	Pass	2:35pm
DET	Pass	2:35pm
BAR	Pass	2:35pm
BT	Pass	2:35pm

Blank Tests

Test	Status	Time
AIR	Pass	2:36pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:36pm

CRC Tests

Test	Status	Time
COMP	Pass	2:36pm
CAL	Pass	2:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSLow Instrument Location JACKSONVILLE
Instrument Serial No. 008930 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 09 day of SEPTEMBER 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY JACKSONVILLE PD 660

Serial Number: 008930

Test Date: 09/09/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034901

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	4:41pm
AIR BLK	.00	4:42pm
ACCY CHK	.07	4:42pm
AIR BLK	.00	4:43pm
SUB TEST	.00	4:46pm
AIR BLK	.00	4:47pm
SUB TEST	.00	4:48pm
AIR BLK	.00	4:49pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY JACKSONVILLE PD 660

Serial Number: 008930 Test Record Number: 2129
Test Date: 09/09/2021 Test Time: 4:50pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:51pm
FLO	Pass	4:51pm
FC	Pass	4:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:51pm
SRC	Pass	4:51pm
DET	Pass	4:51pm
BAR	Pass	4:51pm
BT	Pass	4:51pm

Blank Tests

Test	Status	Time
AIR	Pass	4:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:52pm

CRC Tests

Test	Status	Time
COMP	Pass	4:52pm
CAL	Pass	4:52pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLOW Instrument Location ONSLOW COUNTY
Instrument Serial No. 008931 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931
Test Date: 09/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107401
Exp Date: 03/15/2023

Test	g/210L	Time
DIAG	Pass	12:47pm
AIR BLK	.00	12:48pm
ACCY CHK	.08	12:48pm
AIR BLK	.00	12:50pm
SUB TEST	.00	12:50pm
AIR BLK	.00	12:51pm
SUB TEST	.00	12:52pm
AIR BLK	.00	12:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931 Test Record Number: 3661
Test Date: 09/10/2021 Test Time: 12:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:54pm
FLO	Pass	12:54pm
FC	Pass	12:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:54pm
SRC	Pass	12:54pm
DET	Pass	12:54pm
BAR	Pass	12:54pm
BT	Pass	12:54pm

Blank Tests

Test	Status	Time
AIR	Pass	12:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:55pm

CRC Tests

Test	Status	Time
COMP	Pass	12:55pm
CAL	Pass	12:55pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONslow Instrument Location CAMP LEJEUNE

Instrument Serial No. 008922 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 09 day of SEPTEMBER 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bous
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008922
Test Date: 09/09/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	3:34pm
AIR BLK	.00	3:36pm
ACCY CHK	.07	3:36pm
AIR BLK	.00	3:37pm
SUB TEST	.00	3:38pm
AIR BLK	.00	3:39pm
SUB TEST	.00	3:40pm
AIR BLK	.00	3:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008922 Test Record Number: 529
Test Date: 09/09/2021 Test Time: 3:42pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:42pm
FLO	Pass	3:42pm
FC	Pass	3:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:43pm
SRC	Pass	3:43pm
DET	Pass	3:43pm
BAR	Pass	3:43pm
BT	Pass	3:43pm

Blank Tests

Test	Status	Time
AIR	Pass	3:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:43pm

CRC Tests

Test	Status	Time
COMP	Pass	3:43pm
CAL	Pass	3:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLAW Instrument Location ONSLAW COUNTY
Instrument Serial No. 008932 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Rybens

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008932
Test Date: 09/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	12:48pm
AIR BLK	.00	12:49pm
ACCY CHK	.08	12:50pm
AIR BLK	.00	12:51pm
SUB TEST	.00	12:51pm
AIR BLK	.00	12:52pm
SUB TEST	.00	12:54pm
AIR BLK	.00	12:54pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008932 Test Record Number: 6329
Test Date: 09/10/2021 Test Time: 12:55pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:55pm
FLO	Pass	12:55pm
FC	Pass	12:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:55pm
SRC	Pass	12:55pm
DET	Pass	12:55pm
BAR	Pass	12:55pm
BT	Pass	12:55pm

Blank Tests

Test	Status	Time
AIR	Pass	12:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:56pm

CRC Tests

Test	Status	Time
COMP	Pass	12:56pm
CAL	Pass	12:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County PAMLICO Instrument Location PAMLICO COUNTY

Instrument Serial No. 008640 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Celine R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PAMLICO COUNTY DETENTION CENTER 680

Serial Number: 008640
Test Date: 09/27/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	11:53am
AIR BLK	.00	11:54am
ACCY CHK	.08	11:54am
AIR BLK	.00	11:55am
SUB TEST	.00	11:56am
AIR BLK	.00	11:57am
SUB TEST	.00	11:59am
AIR BLK	.00	11:59am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PAMLICO COUNTY DETENTION CENTER 680

Serial Number: 008640 Test Record Number: 1498
Test Date: 09/27/2021 Test Time: 12:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:00pm
FLO	Pass	12:00pm
FC	Pass	12:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:00pm
SRC	Pass	12:00pm
DET	Pass	12:00pm
BAR	Pass	12:00pm
BT	Pass	12:00pm

Blank Tests

Test	Status	Time
AIR	Pass	12:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:01pm

CRC Tests

Test	Status	Time
COMP	Pass	12:01pm
CAL	Pass	12:01pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Pitt Instrument Location Pitt Co. Detention Center

Instrument Serial No. 008646 124 New Hope Rd, Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646
Test Date: 09/29/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	3:16pm
AIR BLK	.00	3:17pm
ACCY CHK	.08	3:17pm
AIR BLK	.00	3:18pm
SUB TEST	.00	3:19pm
AIR BLK	.00	3:20pm
SUB TEST	.00	3:22pm
AIR BLK	.00	3:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646 Test Record Number: 4277
Test Date: 09/29/2021 Test Time: 3:23pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:24pm
FLO	Pass	3:24pm
FC	Pass	3:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:24pm
SRC	Pass	3:24pm
DET	Pass	3:24pm
BAR	Pass	3:24pm
BT	Pass	3:24pm

Blank Tests

Test	Status	Time
AIR	Pass	3:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:25pm

CRC Tests

Test	Status	Time
COMP	Pass	3:25pm
CAL	Pass	3:25pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Pitt Instrument Location Pitt Co. Detention Center
Instrument Serial No. 008662 174 New Hope Rd, Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662
Test Date: 09/29/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Guard, Kelly G
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018202
Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	3:32pm
AIR BLK	.00	3:33pm
ACCY CHK	.08	3:33pm
AIR BLK	.00	3:34pm
SUB TEST	.00	3:35pm
AIR BLK	.00	3:36pm
SUB TEST	.00	3:38pm
AIR BLK	.00	3:38pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662 Test Record Number: 1233
Test Date: 09/29/2021 Test Time: 3:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:40pm
FLO	Pass	3:40pm
FC	Pass	3:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:40pm
SRC	Pass	3:40pm
DET	Pass	3:40pm
BAR	Pass	3:40pm
BT	Pass	3:40pm

Blank Tests

Test	Status	Time
AIR	Pass	3:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:40pm

CRC Tests

Test	Status	Time
COMP	Pass	3:41pm
CAL	Pass	3:41pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Randolph Instrument Location CAT Mobile Unit 6
Instrument Serial No. 008776 Liberty PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 03 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

660
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY BAT MOBILE UNIT 6 750

Serial Number: 008776
Test Date: 09/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Smith, Jason R
Permit Number: 0024-7428
Effective:
09/29/2020-09/29/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG035001
Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	9:20pm
AIR BLK	.00	9:21pm
ACCY CHK	.07	9:21pm
AIR BLK	.00	9:22pm
SUB TEST	.00	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:26pm
AIR BLK	.00	9:26pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY BAT MOBILE UNIT 6 750

Serial Number: 008776 Test Record Number: 3671
Test Date: 09/03/2021 Test Time: 9:27pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:28pm
FLO	Pass	9:28pm
FC	Pass	9:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:28pm
SRC	Pass	9:28pm
DET	Pass	9:28pm
BAR	Pass	9:28pm
BT	Pass	9:28pm

Blank Tests

Test	Status	Time
AIR	Pass	9:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:28pm

CRC Tests

Test	Status	Time
COMP	Pass	9:29pm
CAL	Pass	9:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROBESON Instrument Location ST. PAULS POLICE
Instrument Serial No. 008814 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27TH day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

667

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY ST PAULS PD 770

Serial Number: 008814
Test Date: 09/27/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number:
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:35am
AIR BLK	.00	11:36am
ACCY CHK	.08	11:36am
AIR BLK	.00	11:38am
SUB TEST	.00	11:39am
AIR BLK	.00	11:40am
SUB TEST	.00	11:41am
AIR BLK	.00	11:42am

Reported AC: .00 g/210L

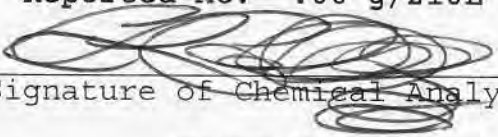
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY ST PAULS PD 770

Serial Number: 008814 Test Record Number: 767
Test Date: 09/27/2021 Test Time: 11:43am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:44am
FLO	Pass	11:44am
FC	Pass	11:44am

Temperature Tests

Test	Status	Time
FC1	Pass	11:44am
SRC	Pass	11:44am
DET	Pass	11:44am
BAR	Pass	11:44am
BT	Pass	11:44am

Blank Tests

Test	Status	Time
AIR	Pass	11:44am


Printer Tests

Test	Status	Time
PRNT	Pass	11:45am

CRC Tests

Test	Status	Time
COMP	Pass	11:45am
CAL	Pass	11:45am

Preventive Maintenance
Status: Pass

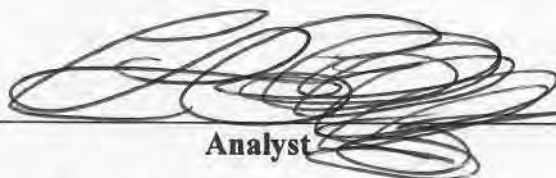
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROWAN Instrument Location SALISBURY POLICE
Instrument Serial No. 008835 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8TH day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835
Test Date: 09/08/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	1:57pm
AIR BLK	.00	1:58pm
ACCY CHK	.08	1:59pm
AIR BLK	.00	2:00pm
SUB TEST	.00	2:00pm
AIR BLK	.00	2:01pm
SUB TEST	.00	2:03pm
AIR BLK	.00	2:04pm

Reported AC: .00 g/210L


Signature of Chemical Analyst
Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835 Test Record Number: 2772
Test Date: 09/08/2021 Test Time: 2:05pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:05pm
FLO	Pass	2:05pm
FC	Pass	2:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:06pm
SRC	Pass	2:06pm
DET	Pass	2:06pm
BAR	Pass	2:06pm
BT	Pass	2:06pm

Blank Tests

Test	Status	Time
AIR	Pass	2:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:06pm

CRC Tests

Test	Status	Time
COMP	Pass	2:06pm
CAL	Pass	2:06pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROWAN Instrument Location CHINA GROVE

Instrument Serial No. 008862 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8TH day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862
Test Date: 09/08/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG107502
Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	1:03pm
AIR BLK	.00	1:04pm
ACCY CHK	.08	1:04pm
AIR BLK	.00	1:05pm
SUB TEST	.00	1:06pm
AIR BLK	.00	1:08pm
SUB TEST	.00	1:09pm
AIR BLK	.00	1:10pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862 Test Record Number: 981
Test Date: 09/08/2021 Test Time: 1:11pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:11pm
FLO	Pass	1:11pm
FC	Pass	1:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:11pm
SRC	Pass	1:11pm
DET	Pass	1:11pm
BAR	Pass	1:11pm
BT	Pass	1:11pm

Blank Tests

Test	Status	Time
AIR	Pass	1:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:12pm

CRC Tests

Test	Status	Time
COMP	Pass	1:12pm
CAL	Pass	1:12pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROWAN Instrument Location SALISBURY POLICE

Instrument Serial No. 008868 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8TH day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868
Test Date: 09/08/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933703
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	2:04pm
AIR BLK	.00	2:05pm
ACCY CHK	.08	2:06pm
AIR BLK	.00	2:07pm
SUB TEST	.00	2:09pm
AIR BLK	.00	2:09pm
SUB TEST	.00	2:11pm
AIR BLK	.00	2:12pm

Reported AC: .00 g/210L


Signature of Chemical Analyst
Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868 Test Record Number: 3290
Test Date: 09/08/2021 Test Time: 2:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:17pm
FLO	Pass	2:17pm
FC	Pass	2:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:17pm
SRC	Pass	2:17pm
DET	Pass	2:17pm
BAR	Pass	2:17pm
BT	Pass	2:17pm

Blank Tests

Test	Status	Time
AIR	Pass	2:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:18pm

CRC Tests

Test	Status	Time
COMP	Pass	2:18pm
CAL	Pass	2:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County SAMPSON Instrument Location SAMPSON COUNTY
Instrument Serial No. 008825 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Basso
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825
Test Date: 09/14/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	5:02pm
AIR BLK	.00	5:03pm
ACCY CHK	.07	5:04pm
AIR BLK	.00	5:05pm
SUB TEST	.00	5:06pm
AIR BLK	.00	5:06pm
SUB TEST	.00	5:08pm
AIR BLK	.00	5:09pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825 Test Record Number: 3279
Test Date: 09/14/2021 Test Time: 5:09pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:10pm
FLO	Pass	5:10pm
FC	Pass	5:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:10pm
SRC	Pass	5:10pm
DET	Pass	5:10pm
BAR	Pass	5:10pm
BT	Pass	5:10pm

Blank Tests

Test	Status	Time
AIR	Pass	5:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:10pm

CRC Tests

Test	Status	Time
COMP	Pass	5:11pm
CAL	Pass	5:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County SAMPSON Instrument Location SAMPSON COUNTY
Instrument Serial No. 008877 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Cheryl Burns

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877
Test Date: 09/14/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG118804
Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	5:13pm
AIR BLK	.00	5:14pm
ACCY CHK	.08	5:14pm
AIR BLK	.00	5:15pm
SUB TEST	.00	5:16pm
AIR BLK	.00	5:17pm
SUB TEST	.00	5:18pm
AIR BLK	.00	5:19pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877 Test Record Number: 3476
Test Date: 09/14/2021 Test Time: 5:19pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:20pm
FLO	Pass	5:20pm
FC	Pass	5:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:20pm
SRC	Pass	5:20pm
DET	Pass	5:20pm
BAR	Pass	5:20pm
BT	Pass	5:20pm

Blank Tests

Test	Status	Time
AIR	Pass	5:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:21pm

CRC Tests

Test	Status	Time
COMP	Pass	5:21pm
CAL	Pass	5:21pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Stanly Instrument Location Locust PD
Instrument Serial No. 008704 Locust, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY LOCUST PD 830

Serial Number: 008706

Test Date: 09/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933901


Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	8:26am
AIR BLK	.00	8:27am
ACCY CHK	.08	8:28am
AIR BLK	.00	8:29am
SUB TEST	.00	8:29am
AIR BLK	.00	8:30am
SUB TEST	.00	8:32am
AIR BLK	.00	8:33am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

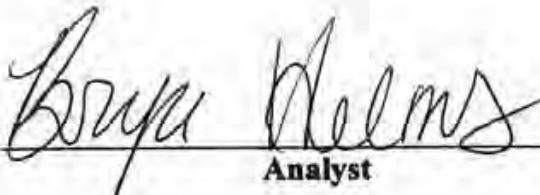
Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY LOCUST PD 830

Serial Number: 008706 Test Record Number: 3600
Test Date: 09/02/2021 Test Time: 8:33am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:33am
FLO	Pass	8:33am
FC	Pass	8:33am

Temperature Tests

Test	Status	Time
FC1	Pass	8:34am
SRC	Pass	8:34am
DET	Pass	8:34am
BAR	Pass	8:34am
BT	Pass	8:34am

Blank Tests

Test	Status	Time
AIR	Pass	8:34am


Printer Tests

Test	Status	Time
PRNT	Pass	8:35am

CRC Tests

Test	Status	Time
COMP	Pass	8:35am
CAL	Pass	8:35am

Preventive Maintenance
Status: *Pass*

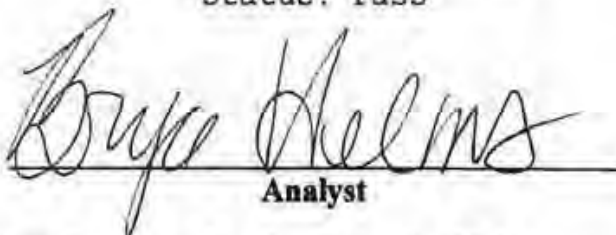
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location Stanly County 80
Albermarle, NC
Instrument Serial No. 008842

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms 674
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842

Test Date: 09/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023


Test	g/210L	Time
DIAG	Pass	9:19am
AIR BLK	.00	9:20am
ACCY CHK	.08	9:21am
AIR BLK	.00	9:22am
SUB TEST	.00	9:22am
AIR BLK	.00	9:23am
SUB TEST	.00	9:25am
AIR BLK	.00	9:25am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

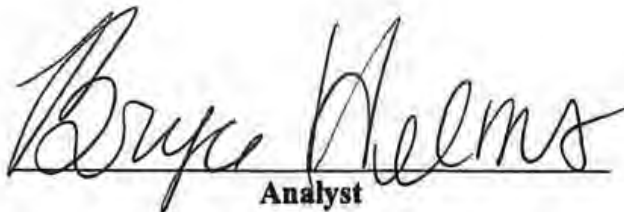

Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842 Test Record Number: 2435
Test Date: 09/02/2021 Test Time: 9:26am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26am
FLO	Pass	9:26am
FC	Pass	9:26am

Temperature Tests

Test	Status	Time
FC1	Pass	9:26am
SRC	Pass	9:26am
DET	Pass	9:26am
BAR	Pass	9:26am
BT	Pass	9:26am

Blank Tests

Test	Status	Time
AIR	Pass	9:27am


Printer Tests

Test	Status	Time
PRNT	Pass	9:27am

CRC Tests

Test	Status	Time
COMP	Pass	9:27am
CAL	Pass	9:27am

Preventive Maintenance
Status: Pass

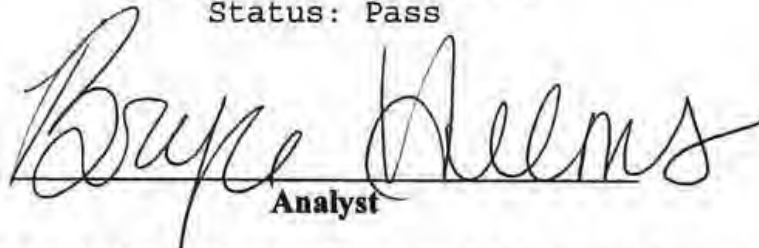
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location Stanly County 80
Albermarle, NC
Instrument Serial No. 008842

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms 674
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842

Test Date: 09/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG107501


Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	9:19am
AIR BLK	.00	9:20am
ACCY CHK	.08	9:21am
AIR BLK	.00	9:22am
SUB TEST	.00	9:22am
AIR BLK	.00	9:23am
SUB TEST	.00	9:25am
AIR BLK	.00	9:25am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

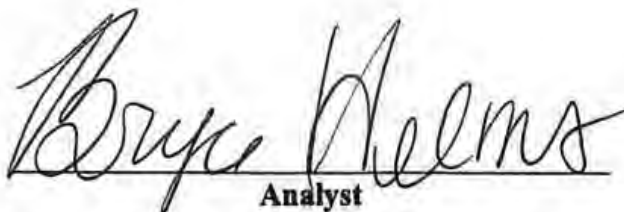
Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842 Test Record Number: 2435
Test Date: 09/02/2021 Test Time: 9:26am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26am
FLO	Pass	9:26am
FC	Pass	9:26am

Temperature Tests

Test	Status	Time
FC1	Pass	9:26am
SRC	Pass	9:26am
DET	Pass	9:26am
BAR	Pass	9:26am
BT	Pass	9:26am

Blank Tests

Test	Status	Time
AIR	Pass	9:27am


Printer Tests

Test	Status	Time
PRNT	Pass	9:27am

CRC Tests

Test	Status	Time
COMP	Pass	9:27am
CAL	Pass	9:27am

Preventive Maintenance
Status: Pass

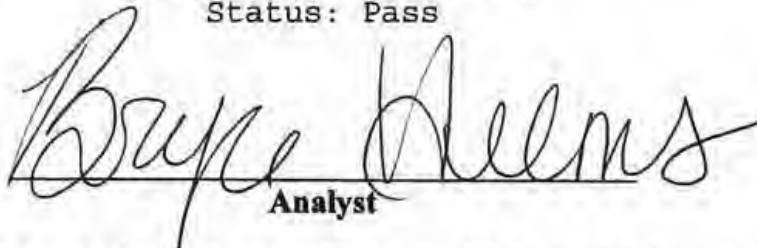
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County STOKES Instrument Location STOKES COUNTY JAIL

Instrument Serial No. 008596 DANBURY, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21ST day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596
Test Date: 09/21/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	11:05am
AIR BLK	.00	11:06am
ACCY CHK	.07	11:06am
AIR BLK	.00	11:07am
SUB TEST	.00	11:08am
AIR BLK	.00	11:09am
SUB TEST	.00	11:10am
AIR BLK	.00	11:11am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596 Test Record Number: 1212
Test Date: 09/21/2021 Test Time: 11:13am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:13am
FLO	Pass	11:13am
FC	Pass	11:13am

Temperature Tests

Test	Status	Time
FC1	Pass	11:13am
SRC	Pass	11:13am
DET	Pass	11:13am
BAR	Pass	11:13am
BT	Pass	11:13am

Blank Tests

Test	Status	Time
AIR	Pass	11:14am


Printer Tests

Test	Status	Time
PRNT	Pass	11:14am

CRC Tests

Test	Status	Time
COMP	Pass	11:14am
CAL	Pass	11:14am

Preventive Maintenance
Status: Pass

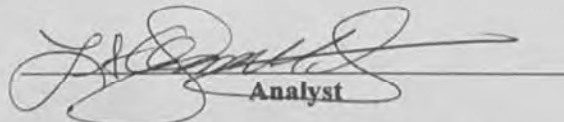
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County STOKES Instrument Location KING POLICE

Instrument Serial No. 008718 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3RD day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY KING P D 840

Serial Number: 008718

Test Date: 09/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	3:05pm
AIR BLK	.00	3:06pm
ACCY CHK	.07	3:07pm
AIR BLK	.00	3:08pm
SUB TEST	.00	3:09pm
AIR BLK	.00	3:10pm
SUB TEST	.00	3:11pm
AIR BLK	.00	3:12pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY KING P D 840

Serial Number: 008718 Test Record Number: 2135
Test Date: 09/03/2021 Test Time: 3:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:13pm
FLO	Pass	3:13pm
FC	Pass	3:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:13pm
SRC	Pass	3:13pm
DET	Pass	3:13pm
BAR	Pass	3:13pm
BT	Pass	3:13pm

Blank Tests

Test	Status	Time
AIR	Pass	3:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:14pm

CRC Tests

Test	Status	Time
COMP	Pass	3:14pm
CAL	Pass	3:14pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Surry Instrument Location Elkin Police
Department
Instrument Serial No. 008926

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy Harbo
Signature of Certifying Official

672
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY ELKIN PD 850

Serial Number: 008926

Test Date: 09/27/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hanks, Timothy S

Permit Number: 0063-3175

Effective:

10/14/2020-10/14/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902


Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:05pm
AIR BLK	.00	1:06pm
ACCY CHK	.08	1:07pm
AIR BLK	.00	1:08pm
SUB TEST	.00	1:08pm
AIR BLK	.00	1:09pm
SUB TEST	.00	1:10pm
AIR BLK	.00	1:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

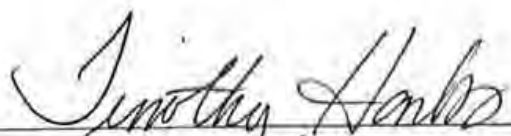
Analyst

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY ELKIN PD 850

Serial Number: 008926 Test Record Number: 992
Test Date: 09/27/2021 Test Time: 1:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:13pm
FLO	Pass	1:13pm
FC	Pass	1:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:13pm
SRC	Pass	1:13pm
DET	Pass	1:13pm
BAR	Pass	1:13pm
BT	Pass	1:13pm

Blank Tests

Test	Status	Time
AIR	Pass	1:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:14pm

CRC Tests

Test	Status	Time
COMP	Pass	1:14pm
CAL	Pass	1:14pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Surry Instrument Location Surry Co Jail
Instrument Serial No. 008934 Dobson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy Horro
Signature of Certifying Official

672
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY SURRY CO JAIL 850

Serial Number: 008934
Test Date: 09/27/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hanks, Timothy S

Permit Number: 0063-3175

Effective:

10/14/2020-10/14/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601


Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:14am
AIR BLK	.00	10:15am
ACCY CHK	.07	10:16am
AIR BLK	.00	10:17am
SUB TEST	.00	10:17am
AIR BLK	.00	10:18am
SUB TEST	.00	10:20am
AIR BLK	.00	10:21am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

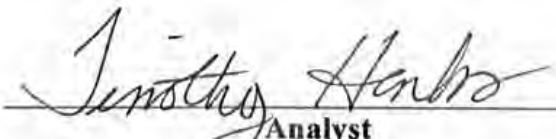
Analyst

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY SURRY CO JAIL 850

Serial Number: 008934 Test Record Number: 2232
Test Date: 09/27/2021 Test Time: 10:32am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:33am
FLO	Pass	10:33am
FC	Pass	10:33am

Temperature Tests

Test	Status	Time
FC1	Pass	10:33am
SRC	Pass	10:33am
DET	Pass	10:33am
BAR	Pass	10:33am
BT	Pass	10:33am

Blank Tests

Test	Status	Time
AIR	Pass	10:34am

Printer Tests

Test	Status	Time
PRNT	Pass	10:34am

CRC Tests

Test	Status	Time
COMP	Pass	10:34am
CAL	Pass	10:34am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County SURRY Instrument Location PIKOT MOUNTAIN

Instrument Serial No. 008938 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3RD day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938

Test Date: 09/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 00

Effective:

00/00/0000-00/00/0000

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	2:16pm
AIR BLK	.00	2:17pm
ACCY CHK	.08	2:18pm
AIR BLK	.00	2:19pm
SUB TEST	.00	2:20pm
AIR BLK	.00	2:20pm
SUB TEST	.00	2:22pm
AIR BLK	.00	2:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938 Test Record Number: 736
Test Date: 09/03/2021 Test Time: 2:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:24pm
FLO	Pass	2:24pm
FC	Pass	2:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:24pm
SRC	Pass	2:24pm
DET	Pass	2:24pm
BAR	Pass	2:24pm
BT	Pass	2:24pm

Blank Tests

Test	Status	Time
AIR	Pass	2:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:25pm

CRC Tests

Test	Status	Time
COMP	Pass	2:25pm
CAL	Pass	2:25pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Surry Instrument Location Mount Airy
Police Department
Instrument Serial No. 008943

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy Henbo
Signature of Certifying Official

672
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943

Test Date: 09/27/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hanks, Timothy S

Permit Number: 0063-3175

Effective:

10/14/2020-10/14/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601


Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:42am
AIR BLK	.00	11:42am
ACCY CHK	.07	11:43am
AIR BLK	.00	11:44am
SUB TEST	.00	11:44am
AIR BLK	.00	11:45am
SUB TEST	.00	11:47am
AIR BLK	.00	11:47am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

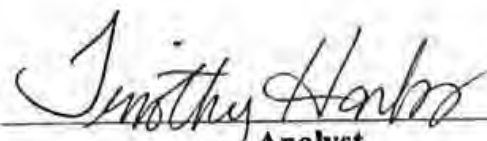
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943 Test Record Number: 2328
Test Date: 09/27/2021 Test Time: 11:49am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:49am
FLO	Pass	11:49am
FC	Pass	11:49am

Temperature Tests

Test	Status	Time
FC1	Pass	11:49am
SRC	Pass	11:49am
DET	Pass	11:49am
BAR	Pass	11:49am
BT	Pass	11:49am

Blank Tests

Test	Status	Time
AIR	Pass	11:50am


Printer Tests

Test	Status	Time
PRNT	Pass	11:50am

CRC Tests

Test	Status	Time
COMP	Pass	11:50am
CAL	Pass	11:50am

Preventive Maintenance
Status: Pass

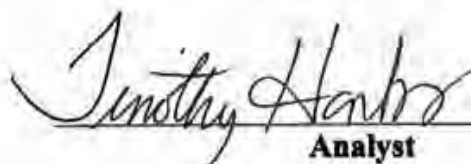

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Stallings PD
Instrument Serial No. 008694 Stallings, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Hulms
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY STALLINGS PD 890

Serial Number: 008694

Test Date: 09/29/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

04/20/2021-04/20/2023

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG035001


Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	8:55am
AIR BLK	.00	8:55am
ACCY CHK	.07	8:56am
AIR BLK	.00	8:57am
SUB TEST	.00	8:58am
AIR BLK	.00	8:59am
SUB TEST	.00	9:00am
AIR BLK	.00	9:01am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY STALLINGS PD 890

Serial Number: 008694 Test Record Number: 1558
Test Date: 09/29/2021 Test Time: 9:01am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:02am
FLO	Pass	9:02am
FC	Pass	9:02am

Temperature Tests

Test	Status	Time
FC1	Pass	9:02am
SRC	Pass	9:02am
DET	Pass	9:02am
BAR	Pass	9:02am
BT	Pass	9:02am

Blank Tests

Test	Status	Time
AIR	Pass	9:03am


Printer Tests

Test	Status	Time
PRNT	Pass	9:03am

CRC Tests

Test	Status	Time
COMP	Pass	9:03am
CAL	Pass	9:03am

Preventive Maintenance
Status: Pass

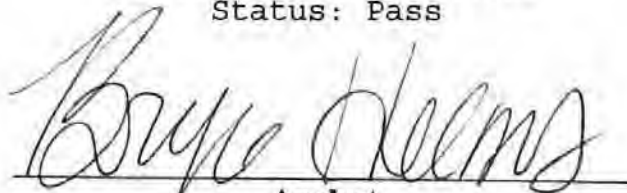

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County WAKE Instrument Location SAT MOBILE UNIT 6
Instrument Serial No. 008580 ZEDULON

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of SEPTEMBER, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

663
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008580

Test Date: 09/17/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Varnell, Bryon L

Permit Number: 0036-1210

Effective:

09/10/2020-09/10/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	8:58pm
AIR BLK	.00	8:59pm
ACCY CHK	.07	8:59pm
AIR BLK	.00	9:00pm
SUB TEST	.00	9:01pm
AIR BLK	.00	9:02pm
SUB TEST	.00	9:03pm
AIR BLK	.00	9:04pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 6 910

Serial Number: 008580 Test Record Number: 2644
Test Date: 09/17/2021 Test Time: 9:05pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:06pm
FLO	Pass	9:06pm
FC	Pass	9:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:06pm
SRC	Pass	9:06pm
DET	Pass	9:06pm
BAR	Pass	9:06pm
BT	Pass	9:06pm

Blank Tests

Test	Status	Time
AIR	Pass	9:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:07pm

CRC Tests

Test	Status	Time
COMP	Pass	9:07pm
CAL	Pass	9:07pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Watauga Instrument Location Watauga Co. Jail
Instrument Serial No. 008715 Boone, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715
Test Date: 09/28/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	10:05am
AIR BLK	.00	10:06am
ACCY CHK	.08	10:06am
AIR BLK	.00	10:07am
SUB TEST	.00	10:08am
AIR BLK	.00	10:09am
SUB TEST	.00	10:10am
AIR BLK	.00	10:11am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715 Test Record Number: 2569
Test Date: 09/28/2021 Test Time: 10:12am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:13am
FLO	Pass	10:13am
FC	Pass	10:13am

Temperature Tests

Test	Status	Time
FC1	Pass	10:13am
SRC	Pass	10:13am
DET	Pass	10:13am
BAR	Pass	10:13am
BT	Pass	10:13am

Blank Tests

Test	Status	Time
AIR	Pass	10:13am


Printer Tests

Test	Status	Time
PRNT	Pass	10:14am

CRC Tests

Test	Status	Time
COMP	Pass	10:14am
CAL	Pass	10:14am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Knightsdale PD
Instrument Serial No. 008838 879 Stangle Square Ct
Knightsdale, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of September, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ed Bryant
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: 008838

Test Date: 09/07/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG118804

Exp Date: 07/07/2023

Test	g/210L	Time
DIAG	Pass	11:34am
AIR BLK	.00	11:34am
ACCY CHK	.07	11:35am
AIR BLK	.00	11:36am
SUB TEST	.00	11:36am
AIR BLK	.00	11:37am
SUB TEST	.00	11:39am
AIR BLK	.00	11:39am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: 008838 Test Record Number: 2161
Test Date: 09/07/2021 Test Time: 11:40am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41am
FLO	Pass	11:41am
FC	Pass	11:41am

Temperature Tests

Test	Status	Time
FC1	Pass	11:41am
SRC	Pass	11:41am
DET	Pass	11:41am
BAR	Pass	11:41am
BT	Pass	11:41am

Blank Tests

Test	Status	Time
AIR	Pass	11:41am

Printer Tests

Test	Status	Time
PRNT	Pass	11:41am

CRC Tests

Test	Status	Time
COMP	Pass	11:41am
CAL	Pass	11:41am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilson Instrument Location Wilson Co. Detention Center
Instrument Serial No. 008627 100 E. Green St, Wilson, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key Q
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627
Test Date: 09/21/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	9:57am
AIR BLK	.00	9:58am
ACCY CHK	.08	9:59am
AIR BLK	.00	10:00am
SUB TEST	.00	10:00am
AIR BLK	.00	10:01am
SUB TEST	.00	10:03am
AIR BLK	.00	10:04am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627 Test Record Number: 2864
Test Date: 09/21/2021 Test Time: 10:04am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:05am
FLO	Pass	10:05am
FC	Pass	10:05am

Temperature Tests

Test	Status	Time
FC1	Pass	10:05am
SRC	Pass	10:05am
DET	Pass	10:05am
BAR	Pass	10:05am
BT	Pass	10:05am

Blank Tests

Test	Status	Time
AIR	Pass	10:06am

Printer Tests

Test	Status	Time
PRNT	Pass	10:06am

CRC Tests

Test	Status	Time
COMP	Pass	10:06am
CAL	Pass	10:06am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilson Instrument Location Wilson Co. Detention Center
Instrument Serial No. 008652 100 E Green St, Wilson, N.C

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6043
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652
Test Date: 09/21/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG107501

Exp Date: 03/16/2023

Test	g/210L	Time
DIAG	Pass	9:48am
AIR BLK	.00	9:49am
ACCY CHK	.08	9:49am
AIR BLK	.00	9:51am
SUB TEST	.00	9:51am
AIR BLK	.00	9:52am
SUB TEST	.00	9:54am
AIR BLK	.00	9:55am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652 Test Record Number: 3592
Test Date: 09/21/2021 Test Time: 9:56am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:56am
FLO	Pass	9:56am
FC	Pass	9:56am

Temperature Tests

Test	Status	Time
FC1	Pass	9:56am
SRC	Pass	9:56am
DET	Pass	9:56am
BAR	Pass	9:56am
BT	Pass	9:56am

Blank Tests

Test	Status	Time
AIR	Pass	9:57am


Printer Tests

Test	Status	Time
PRNT	Pass	9:57am

CRC Tests

Test	Status	Time
COMP	Pass	9:57am
CAL	Pass	9:57am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Yancey Instrument Location Yancey County Jail

Instrument Serial No. 009653 Blountville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of September, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

YANCEY COUNTY YANCEY COUNTY JAIL 990

Serial Number: 008653
Test Date: 09/02/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018401

Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	11:39am
AIR BLK	.00	11:40am
ACCY CHK	.07	11:40am
AIR BLK	.00	11:41am
SUB TEST	.00	11:42am
AIR BLK	.00	11:43am
SUB TEST	.00	11:45am
AIR BLK	.00	11:46am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

YANCEY COUNTY YANCEY COUNTY JAIL 990

Serial Number: 008653 Test Record Number: 1562
Test Date: 09/02/2021 Test Time: 11:47am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:47am
FLO	Pass	11:47am
FC	Pass	11:48am

Temperature Tests

Test	Status	Time
FC1	Pass	11:48am
SRC	Pass	11:48am
DET	Pass	11:48am
BAR	Pass	11:48am
BT	Pass	11:48am

Blank Tests

Test	Status	Time
AIR	Pass	11:48am

Printer Tests

Test	Status	Time
PRNT	Pass	11:48am

CRC Tests

Test	Status	Time
COMP	Pass	11:48am
CAL	Pass	11:48am

Preventive Maintenance
Status: Pass



Analyst